

LB105234

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/19/2019 14:43


Test Phenolics-

Accepted 9/19/2019 14:43

Factor 9.029
Bias 0.009

Coeff. of det. 0.999957

Errors

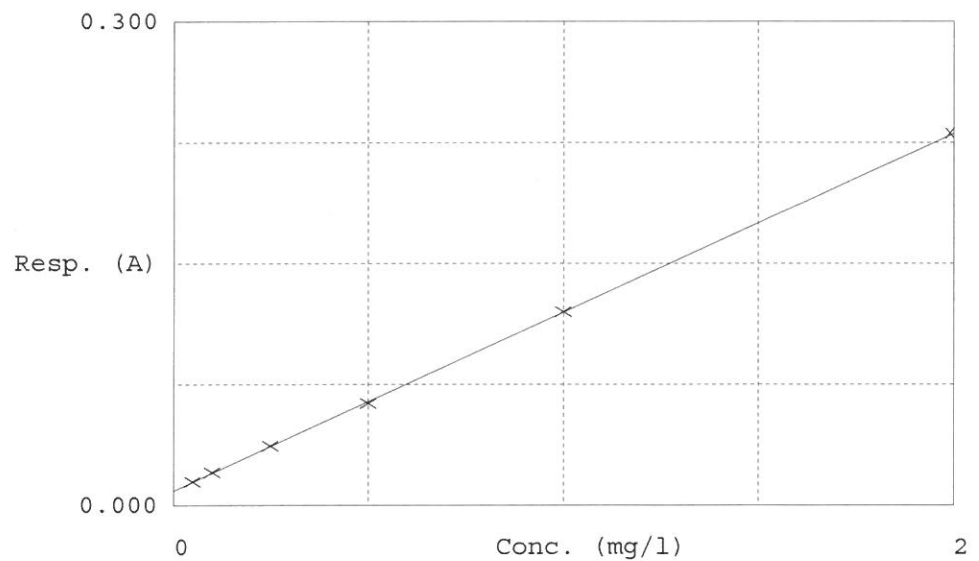

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.015	0.0515	0.0500	
2	Phenol-2	0.021	0.1033	0.1000	
3	Phenol-2	0.037	0.2521	0.2500	
4	Phenol-2	0.063	0.4902	0.5000	
5	Phenol-2	0.120	1.0019	1.0000	
6	Phenol-2	0.231	2.0010	2.0000	

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/19/2019 15:56

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.989	0.0	0.119	
ICB1	0.001	0.0	0.009	
CCV1	1.025	0.0	0.123	
CCB1	0.005	0.0	0.010	
PB123217BL	0.003	0.0	0.009	
PB123217BS	0.993	0.0	0.119	
K4843-27	1.581	0.0	0.184	
CCV2	1.004	0.0	0.120	
CCB2	0.003	0.0	0.009	

N	9
Mean	0.623
SD	0.6157
CV%	98.87

9/19/19
CT

Aquakem v. 7.2AQ1

Results from time period:

Thu Sep 19 14:19:09 2019

Thu Sep 19 15:13:15 2019

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0515	mg/l	9/19/2019 14:42:43	
0.1PPM	A	Phenolics-	P	0.1033	mg/l	9/19/2019 14:42:44	
0.25PPM	A	Phenolics-	P	0.2521	mg/l	9/19/2019 14:42:45	
0.50PPM	A	Phenolics-	P	0.4902	mg/l	9/19/2019 14:42:46	
1.0PPM	A	Phenolics-	P	1.0019	mg/l	9/19/2019 14:42:47	
2.0PPM	A	Phenolics-	P	2.001	mg/l	9/19/2019 14:42:48	
ICV1	S	Phenolics-	P	0.989	mg/l	9/19/2019 15:13:04	
ICB1	S	Phenolics-	P	0.0007	mg/l	9/19/2019 15:13:05	
CCV1	S	Phenolics-	P	1.0246	mg/l	9/19/2019 15:13:06	
CCB1	S	Phenolics-	P	0.0051	mg/l	9/19/2019 15:13:07	
PB123217BL	S	Phenolics-	P	0.0034	mg/l	9/19/2019 15:13:08	
PB123217BS	S	Phenolics-	P	0.9927	mg/l	9/19/2019 15:13:09	
K4843-27	S	Phenolics-	P	1.5814	mg/l	9/19/2019 15:13:10	
CCV2	S	Phenolics-	P	1.0043	mg/l	9/19/2019 15:13:13	
CCB2	S	Phenolics-	P	0.0033	mg/l	9/19/2019 15:13:14	