

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CS

Instrument ID : Konelab

9/19/2019 16:26

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.002	0.0	0.120	
ICB1	0.011	0.0	0.010	
CCV1	1.023	0.0	0.122	
CCB1	0.010	0.0	0.010	
PB123218BL	0.006	0.0	0.010	
PB123218BS	1.023	0.0	0.122	
K4843-26	1.611	0.0	0.188	
CCV2	1.030	0.0	0.123	
CCB2	0.010	0.0	0.010	

N	9
Mean	0.636
SD	0.6236
CV%	98.00

18109235

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : CT

Instrument ID : Konelab

9/19/2019 14:43


Test Phenolics-

Accepted 9/19/2019 14:43

Factor 9.029
 Bias 0.009

Coeff. of det. 0.999957

Errors

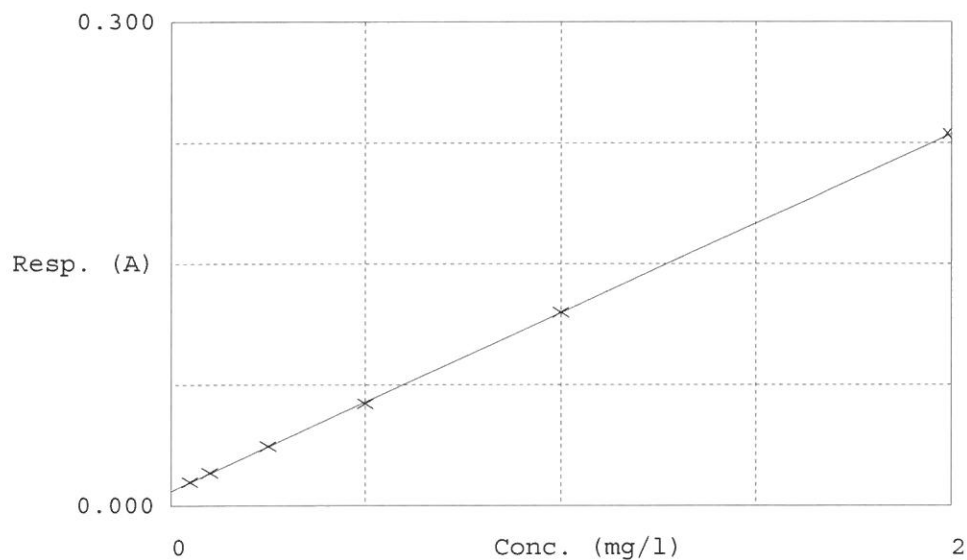

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.015	0.0515	0.0500	
2	Phenol-2	0.021	0.1033	0.1000	
3	Phenol-2	0.037	0.2521	0.2500	
4	Phenol-2	0.063	0.4902	0.5000	
5	Phenol-2	0.120	1.0019	1.0000	
6	Phenol-2	0.231	2.0010	2.0000	

01/19/19

CT

Aquakem v. 7.2AQ1

Results from time period:

Thu Sep 19 16:20:37 2019

Thu Sep 19 16:20:45 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0515	mg/l	9/19/2019 14:42:43	
0.1PPM	A	Phenolics-	P	0.1033	mg/l	9/19/2019 14:42:44	
0.25PPM	A	Phenolics-	P	0.2521	mg/l	9/19/2019 14:42:45	
0.50PPM	A	Phenolics-	P	0.4902	mg/l	9/19/2019 14:42:46	
1.0PPM	A	Phenolics-	P	1.0019	mg/l	9/19/2019 14:42:47	
2.0PPM	A	Phenolics-	P	2.001	mg/l	9/19/2019 14:42:48	
ICV1	S	Phenolics-	P	1.0025	mg/l	9/19/2019 16:20:37	
ICB1	S	Phenolics-	P	0.0115	mg/l	9/19/2019 16:20:38	
CCV1	S	Phenolics-	P	1.0231	mg/l	9/19/2019 16:20:39	
CCB1	S	Phenolics-	P	0.01	mg/l	9/19/2019 16:20:40	
PB123218BL	S	Phenolics-	P	0.0056	mg/l	9/19/2019 16:20:41	
PB123218BS	S	Phenolics-	P	1.023	mg/l	9/19/2019 16:20:42	
K4843-26	S	Phenolics-	P	1.6113	mg/l	9/19/2019 16:20:43	
CCV2	S	Phenolics-	P	1.0296	mg/l	9/19/2019 16:20:44	
CCB2	S	Phenolics-	P	0.0103	mg/l	9/19/2019 16:20:45	