

LB105250

=====

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : CT

Instrument ID : Konelab

9/20/2019 8:42


Test Total CN

Accepted 9/20/2019 8:42

Factor 1064
Bias 0.001

Coeff. of det. 0.998950

Errors

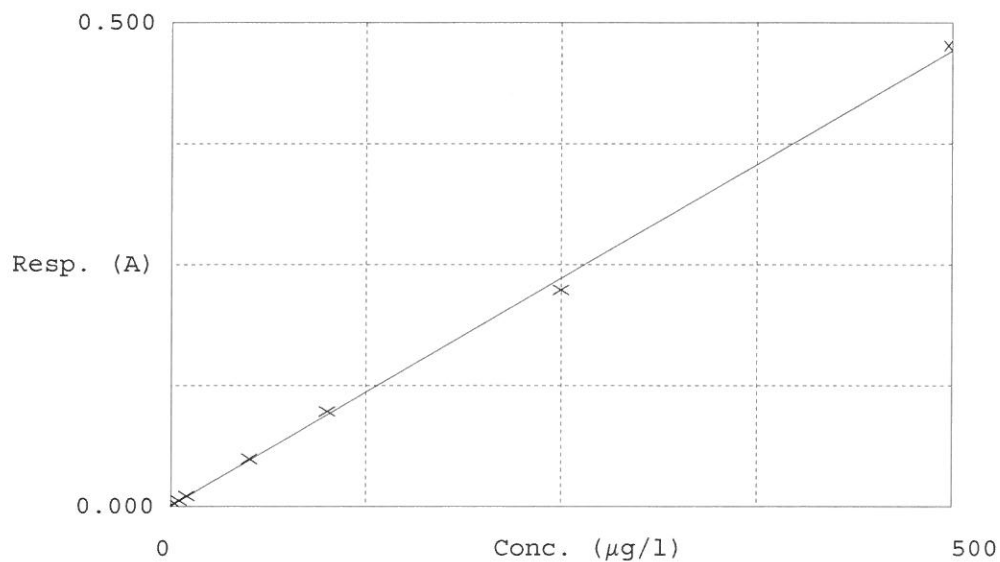

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.6653	0.0000	
2	5.0PPBCN	0.006	5.7959	5.0000	
3	10PPBCN	0.011	10.8886	10.0000	
4	50PPBCN	0.049	51.4056	50.0000	
5	100PPBCN	0.098	103.6132	100.0000	
6	250PPBCN	0.224	237.0406	250.0000	
7	500PPBCN	0.476	505.5907	500.0000	

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/20/2019 9:22

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.329	0.0	0.093	
ICB1	0.755	0.0	0.002	
CCV1	226.364	0.0	0.214	
CCB1	0.681	0.0	0.002	
PB123235BL	0.474	0.0	0.001	
PB123235BS	99.230	0.0	0.094	
MIDPB123235	228.454	0.0	0.216	
K4788-01	2.516	0.0	0.003	
K4788-01DUP	2.378	0.0	0.003	
K4788-01MS	48.216	0.0	0.046	
K4788-01MSD	47.619	0.0	0.046	
K4973-01	0.691	0.0	0.002	
CCV2	237.540	0.0	0.224	
CCB2	0.827	0.0	0.002	

N	14
Mean	71.005
SD	93.3952
CV%	131.53

9/20/19
CT

Aquakem v. 7.2AQ1

Results from time period:

Fri Sep 20 08:19:55 2019

Fri Sep 20 09:19:57 2019

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.6653	µg/l	9/20/2019 8:40:41	
5.0PPBCN	A	Total CN	P	5.7959	µg/l	9/20/2019 8:40:42	
10PPBCN	A	Total CN	P	10.8886	µg/l	9/20/2019 8:40:43	
50PPBCN	A	Total CN	P	51.4056	µg/l	9/20/2019 8:40:44	
100PPBCN	A	Total CN	P	103.6132	µg/l	9/20/2019 8:40:45	
250PPBCN	A	Total CN	P	237.0406	µg/l	9/20/2019 8:40:46	
500PPBCN	A	Total CN	P	505.5907	µg/l	9/20/2019 8:40:47	
ICV1	S	Total CN	P	98.3294	µg/l	9/20/2019 9:15:35	
ICB1	S	Total CN	P	0.7555	µg/l	9/20/2019 9:15:36	
CCV1	S	Total CN	P	226.3645	µg/l	9/20/2019 9:15:37	
CCB1	S	Total CN	P	0.681	µg/l	9/20/2019 9:15:38	
PB123235BL	S	Total CN	P	0.4741	µg/l	9/20/2019 9:15:39	
PB123235BS	S	Total CN	P	99.2301	µg/l	9/20/2019 9:15:40	
MIDPB123235	S	Total CN	P	228.4541	µg/l	9/20/2019 9:15:41	
K4788-01	S	Total CN	P	2.5164	µg/l	9/20/2019 9:15:42	
K4788-01DUP	S	Total CN	P	2.3785	µg/l	9/20/2019 9:15:43	
K4788-01MS	S	Total CN	P	48.2164	µg/l	9/20/2019 9:15:44	
K4788-01MSD	S	Total CN	P	47.6191	µg/l	9/20/2019 9:15:45	
K4973-01	S	Total CN	P	0.6908	µg/l	9/20/2019 9:19:54	
CCV2	S	Total CN	P	237.54	µg/l	9/20/2019 9:19:55	
CCB2	S	Total CN	P	0.8267	µg/l	9/20/2019 9:19:56	