

LB105284

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : CT

Instrument ID : Konelab

9/23/2019 11:36


Test ^{Reactive}
~~Total~~ CN

Accepted 9/23/2019 11:36

Factor 1167
 Bias 0.002

Coeff. of det. 0.999846

Errors

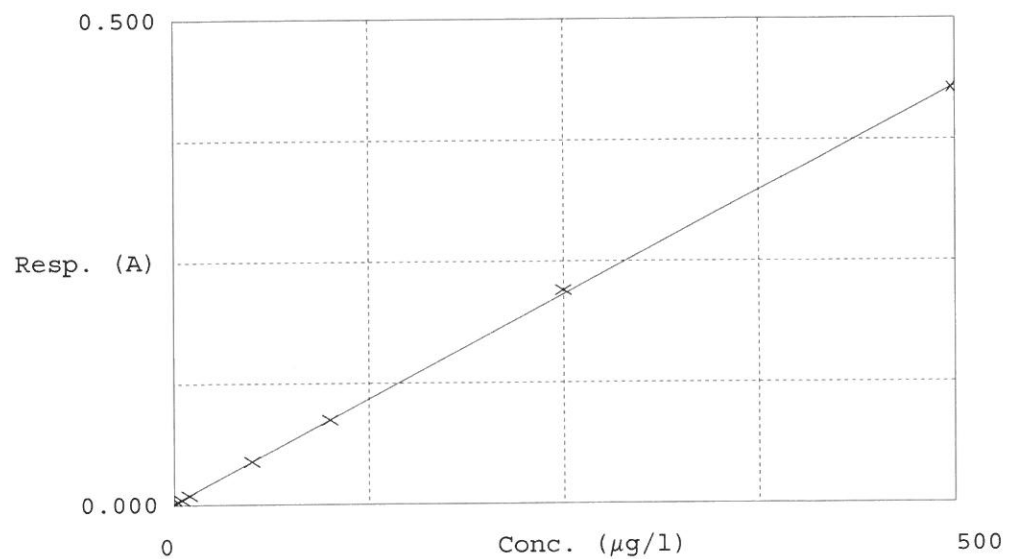

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.6739	0.0000	
2	5.0PPBCN	0.005	4.0778	5.0000	
3	10PPBCN	0.010	9.2071	10.0000	
4	50PPBCN	0.045	49.9109	50.0000	
5	100PPBCN	0.088	100.0036	100.0000	
6	250PPBCN	0.220	254.8827	250.0000	
7	500PPBCN	0.428	497.5920	500.0000	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/23/2019 12:09

Test: ^{Reactive}
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.491	0.0	0.085	
ICB1	-0.391	0.0	0.001	
CCV1	245.010	0.0	0.212	
CCB1	1.017	0.0	0.003	
PB123294BL	-0.601	0.0	0.001	
K4665-06	-0.419	0.0	0.001	
K4997-11	-0.626	0.0	0.001	
K4997-11DUP	-0.736	0.0	0.001	
K4997-13	-0.516	0.0	0.001	
K4997-15	-0.042	0.0	0.002	
K4997-17	-0.615	0.0	0.001	
K4997-19	-2.644	0.0	-0.000	
CCV2	262.747	0.0	0.227	
CCB2	-0.188	0.0	0.002	

N	14
Mean	42.820
SD	93.1957
CV%	217.64

9/23/19
CT

Aquakem v. 7.2AQ1

Results from time period:

Mon Sep 23 11:33:45 2019

Mon Sep 23 12:07:17 2019

Sample Id	Sam/Ctr/c	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.6739	µg/l	9/23/2019 11:33:45	
5.0PPBCN	A	Reactive CN	P	4.0778	µg/l	9/23/2019 11:33:46	
10PPBCN	A	Reactive CN	P	9.2071	µg/l	9/23/2019 11:33:47	
50PPBCN	A	Reactive CN	P	49.9109	µg/l	9/23/2019 11:33:48	
100PPBCN	A	Reactive CN	P	100.0036	µg/l	9/23/2019 11:33:49	
250PPBCN	A	Reactive CN	P	254.8827	µg/l	9/23/2019 11:33:50	
500PPBCN	A	Reactive CN	P	497.592	µg/l	9/23/2019 11:33:51	
ICV1	S	Reactive CN	P	97.4914	µg/l	9/23/2019 12:03:24	
ICB1	S	Reactive CN	P	-0.391	µg/l	9/23/2019 12:03:25	
CCV1	S	Reactive CN	P	245.0099	µg/l	9/23/2019 12:03:26	
CCB1	S	Reactive CN	P	1.0165	µg/l	9/23/2019 12:03:27	
PB123294BL	S	Reactive CN	P	-0.601	µg/l	9/23/2019 12:03:28	
K4665-06	S	Reactive CN	P	-0.4187	µg/l	9/23/2019 12:03:29	
K4997-11	S	Reactive CN	P	-0.6264	µg/l	9/23/2019 12:03:30	
K4997-11DUP	S	Reactive CN	P	-0.7362	µg/l	9/23/2019 12:03:31	
K4997-13	S	Reactive CN	P	-0.5158	µg/l	9/23/2019 12:03:32	
K4997-15	S	Reactive CN	P	-0.0422	µg/l	9/23/2019 12:03:33	
K4997-17	S	Reactive CN	P	-0.6151	µg/l	9/23/2019 12:03:34	
K4997-19	S	Reactive CN	P	-2.6436	µg/l	9/23/2019 12:07:15	
CCV2	S	Reactive CN	P	262.7473	µg/l	9/23/2019 12:07:16	
CCB2	S	Reactive CN	P	-0.1884	µg/l	9/23/2019 12:07:17	