


LB105305

7471B

INSTRUMENT ID : CU1

Linear

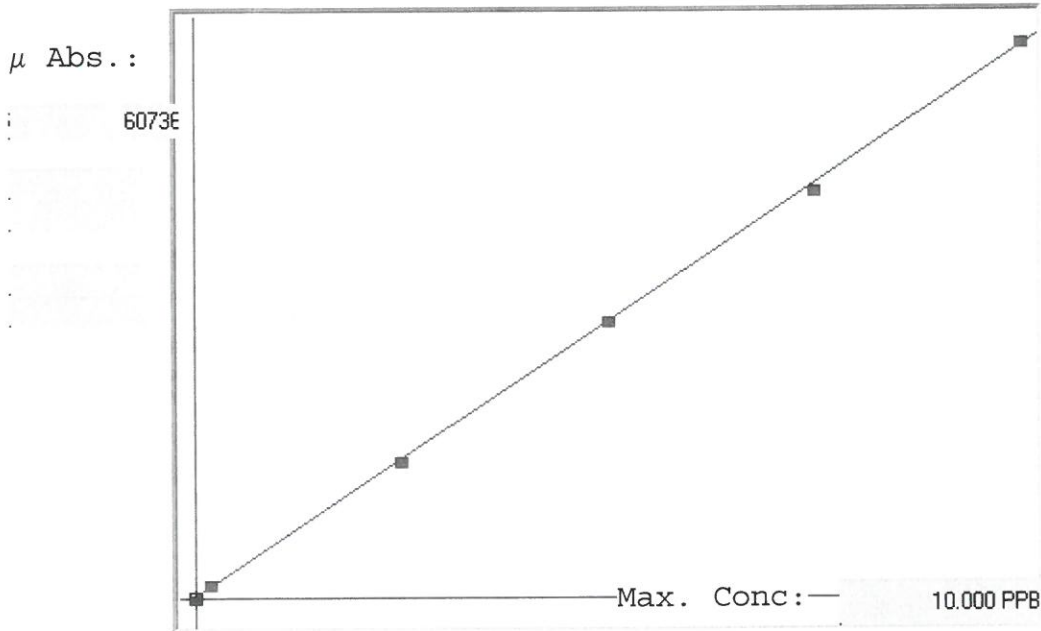

A= 0.0000e+000

B= 1.6590e-004

C= -1.2716e-002

Rho= 0.9999084

Accept = Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.003	-0.003	61	0.000	61				
0.2	0.200	0.244	0.044	1546	0.0 %	1546				
2.5	2.500	2.466	-0.034	14944	0.0 %	14944				
5.0	5.000	5.016	0.016	30314	0.0 %	30314				
7.5	7.500	7.413	-0.087	44758	0.0 %	44758				
10.0	10.000	10.063	0.063	60736	0.0 %	60736				

LB105305 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 24 Sep 2019 14:35:31

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50-0	61	-	0.00007471B	PPB	24 Sep 2019 14:40:22	S	Std
0.2 - 1	50-2	1546	-	0.20007471B	PPB	24 Sep 2019 14:42:40	S	Std
2.5 - 1	52-5	14944	-	2.50007471B	PPB	24 Sep 2019 14:44:58	S	Std
5.0 - 1	55-0	30314	-	5.00007471B	PPB	24 Sep 2019 14:47:16	S	Std
7.5 - 1	57-5	44758	-	7.50007471B	PPB	24 Sep 2019 14:49:33	S	Std
10.0 - 1	510-0	60736	-	10.00007471B	PPB	24 Sep 2019 14:51:51	S	Std
ICV27 - 1	ICV27	24129	3.9903	-7471B	PPB	24 Sep 2019 14:57:03	U	SMPL
ICB27 - 1	ICB27	190	0.0188	-7471B	PPB	24 Sep 2019 14:59:19	U	SMPL
CCV02 - 1	CCV02	30614	5.0661	-7471B	PPB	24 Sep 2019 15:01:36	U	SMPL
CCB02 - 1	CCB02	65	-0.0019	-7471B	PPB	24 Sep 2019 15:03:53	U	SMPL
CRA - 1	CRA	1552	0.2448	-7471B	PPB	24 Sep 2019 15:06:09	U	SMPL
HighStd - 1	HighStd	60280	9.9877	-7471B	PPB	24 Sep 2019 15:08:25	U	SMPL
ChkStd - 1	ChkStd	41763	6.9157	-7471B	PPB	24 Sep 2019 15:10:41	U	SMPL
PB123361BL - 1	PBS	37	-0.0066	-7471B	PPB	24 Sep 2019 15:12:59	U	SMPL
PB123361BS - 1	LCSS	21526	3.5584	-7471B	PPB	24 Sep 2019 15:15:16	U	SMPL
K4664-10 - 1	OR-03-092319	3501	0.5681	-7471B	PPB	24 Sep 2019 15:17:33	U	SMPL
K4664-10DUP - 1	OR-03-092319DUP	3615	0.5870	-7471B	PPB	24 Sep 2019 15:19:52	U	SMPL
K4664-10MS - 1	OR-03-092319MS	25009	4.1363	-7471B	PPB	24 Sep 2019 15:28:39	U	SMPL
K4664-10MSD - 1	OR-03-092319MSD	26751	4.4253	-7471B	PPB	24 Sep 2019 15:30:57	U	SMPL
K4665-01 - 1	EO-01-091919	7049	1.1567	-7471B	PPB	24 Sep 2019 15:33:14	U	SMPL
CCV03 - 1	CCV03	30515	5.0497	-7471B	PPB	24 Sep 2019 15:35:31	U	SMPL
CCB03 - 1	CCB03	77	0.0001	-7471B	PPB	24 Sep 2019 15:37:48	U	SMPL
K4668-12 - 1	SU-03-092319	5102	0.8337	-7471B	PPB	24 Sep 2019 15:40:06	U	SMPL
K4980-04 - 1	SAND-STOCKPILE-1	2355	0.3780	-7471B	PPB	24 Sep 2019 15:42:24	U	SMPL
K4997-01 - 1	WC-08-091919	13835	2.2825	-7471B	PPB	24 Sep 2019 15:44:40	U	SMPL
K4997-03 - 1	WC-09-091919	11194	1.8444	-7471B	PPB	24 Sep 2019 15:46:57	U	SMPL
K4997-05 - 1	WC-10-091919	11572	1.9071	-7471B	PPB	24 Sep 2019 15:49:14	U	SMPL
K4997-07 - 1	WC-11-091919	8408	1.3822	-7471B	PPB	24 Sep 2019 15:51:32	U	SMPL
K4997-09 - 1	WC-12-091919	6588	1.0802	-7471B	PPB	24 Sep 2019 15:53:49	U	SMPL
K5008-01 - 1	SB-1	4741	0.7738	-7471B	PPB	24 Sep 2019 15:56:06	U	SMPL
K5008-02 - 1	SB-2	6850	1.1237	-7471B	PPB	24 Sep 2019 15:58:24	U	SMPL
K5008-03 - 1	SB-3	5536	0.9057	-7471B	PPB	24 Sep 2019 16:00:40	U	SMPL
CCV04 - 1	CCV04	30627	5.0683	-7471B	PPB	24 Sep 2019 16:02:56	U	SMPL
CCB04 - 1	CCB04	28	-0.0081	-7471B	PPB	24 Sep 2019 16:05:12	U	SMPL
K5008-04 - 1	SB-4	403	0.0541	-7471B	PPB	24 Sep 2019 16:07:28	U	SMPL
K5008-05 - 1	SB-5	5855	0.9586	-7471B	PPB	24 Sep 2019 16:09:44	U	SMPL
K5008-06 - 1	SB-6	4236	0.6900	-7471B	PPB	24 Sep 2019 16:12:00	U	SMPL
K5008-07 - 1	SB-7	1998	0.3188	-7471B	PPB	24 Sep 2019 16:14:16	U	SMPL
K5008-08 - 1	SB-8	4385	0.7148	-7471B	PPB	24 Sep 2019 16:16:34	U	SMPL
K5008-09 - 1	SB-9	1709	0.2708	-7471B	PPB	24 Sep 2019 16:18:51	U	SMPL
K5010-03 - 1	BSP-2	5715	0.9354	-7471B	PPB	24 Sep 2019 16:21:08	U	SMPL
K4664-10LX5 - 1		710	0.1051	-7471B	PPB	24 Sep 2019 16:23:25	U	SMPL
K4664-10A - 1		25043	4.1419	-7471B	PPB	24 Sep 2019 16:25:43	U	SMPL
CCV05 - 1	CCV05	30495	5.0464	-7471B	PPB	24 Sep 2019 16:27:59	U	SMPL
CCB05 - 1	CCB05	78	0.0002	-7471B	PPB	24 Sep 2019 16:30:16	U	SMPL