

LB105312

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/25/2019 9:19


Test ^{Reactive}
~~Total~~ CN

Accepted 9/25/2019 9:19

Factor 1188
Bias 0.001

Coeff. of det. 0.999962

Errors

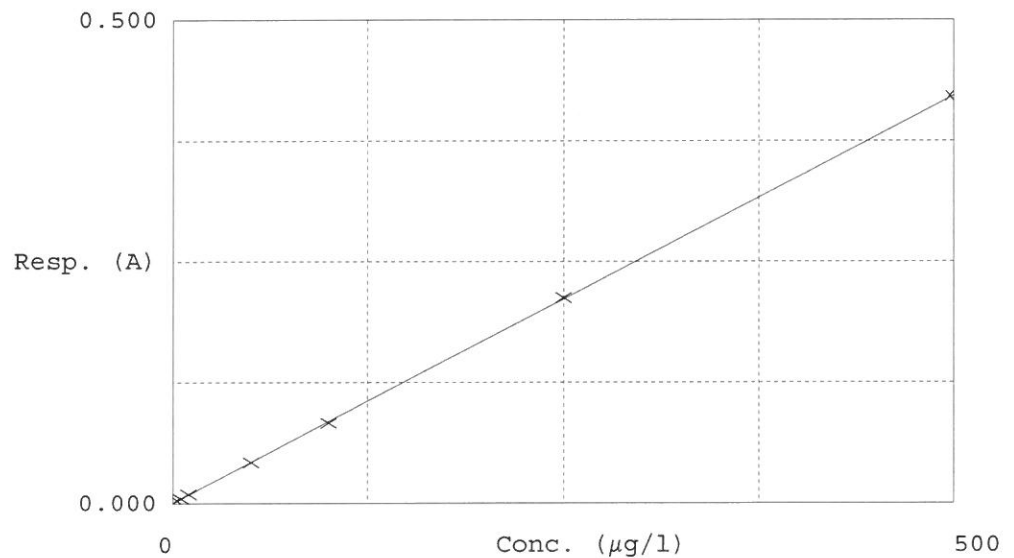

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.7002	0.0000	
2	5.0PPBCN	0.005	5.0530	5.0000	
3	10PPBCN	0.010	10.4967	10.0000	
4	50PPBCN	0.042	49.5428	50.0000	
5	100PPBCN	0.083	97.9687	100.0000	
6	250PPBCN	0.213	251.5939	250.0000	
7	500PPBCN	0.421	499.6445	500.0000	

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/25/2019 9:56

Reactive

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.395	0.0	0.081	
ICB1	1.146	0.0	0.002	
CCV1	237.560	0.0	0.201	
CCB1	0.070	0.0	0.001	
PB123348BL	0.843	0.0	0.001	
K4664-13	0.874	0.0	0.002	
K4664-13DUP	0.551	0.0	0.001	
K4664-15 K4668-15	0.683	0.0	0.001	
K5010-01	0.414	0.0	0.001	
CCV2	240.978	0.0	0.204	
CCB2	0.880	0.0	0.002	

N	11
Mean	52.672
SD	96.4842
CV%	183.18

CT
9/25/19

Aquakem v. 7.2AQ1

Results from time period:

Wed Sep 25 08:41:06 2019

Wed Sep 25 09:47:05 2019

Sample Id	Sam/Ctr/c	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	0.7002	µg/l	9/25/2019 9:15:10	
5.0PPBCN	A	Reactive CN	P	5.053	µg/l	9/25/2019 9:15:11	
10PPBCN	A	Reactive CN	P	10.4967	µg/l	9/25/2019 9:15:12	
50PPBCN	A	Reactive CN	P	49.5428	µg/l	9/25/2019 9:15:13	
100PPBCN	A	Reactive CN	P	97.9687	µg/l	9/25/2019 9:15:14	
250PPBCN	A	Reactive CN	P	251.5939	µg/l	9/25/2019 9:15:15	
500PPBCN	A	Reactive CN	P	499.6445	µg/l	9/25/2019 9:15:16	
ICV1	S	Reactive CN	P	95.3952	µg/l	9/25/2019 9:46:55	
ICB1	S	Reactive CN	P	1.1463	µg/l	9/25/2019 9:46:56	
CCV1	S	Reactive CN	P	237.5604	µg/l	9/25/2019 9:46:57	
CCB1	S	Reactive CN	P	0.0696	µg/l	9/25/2019 9:46:58	
PB123348BL	S	Reactive CN	P	0.8426	µg/l	9/25/2019 9:46:59	
K4664-13	S	Reactive CN	P	0.8741	µg/l	9/25/2019 9:47:00	
K4664-13DUP	S	Reactive CN	P	0.5512	µg/l	9/25/2019 9:47:01	
K4668-15	S	Reactive CN	P	0.6827	µg/l	9/25/2019 9:47:02	
K5010-01	S	Reactive CN	P	0.4143	µg/l	9/25/2019 9:47:03	
CCV2	S	Reactive CN	P	240.9777	µg/l	9/25/2019 9:47:04	
CCB2	S	Reactive CN	P	0.8797	µg/l	9/25/2019 9:47:05	