

LB105329

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : CT

Instrument ID : Konelab

9/26/2019 8:23


Test Total CN

Accepted 9/26/2019 8:23

Factor 1185
Bias 0.001

Coeff. of det. 0.999969

Errors

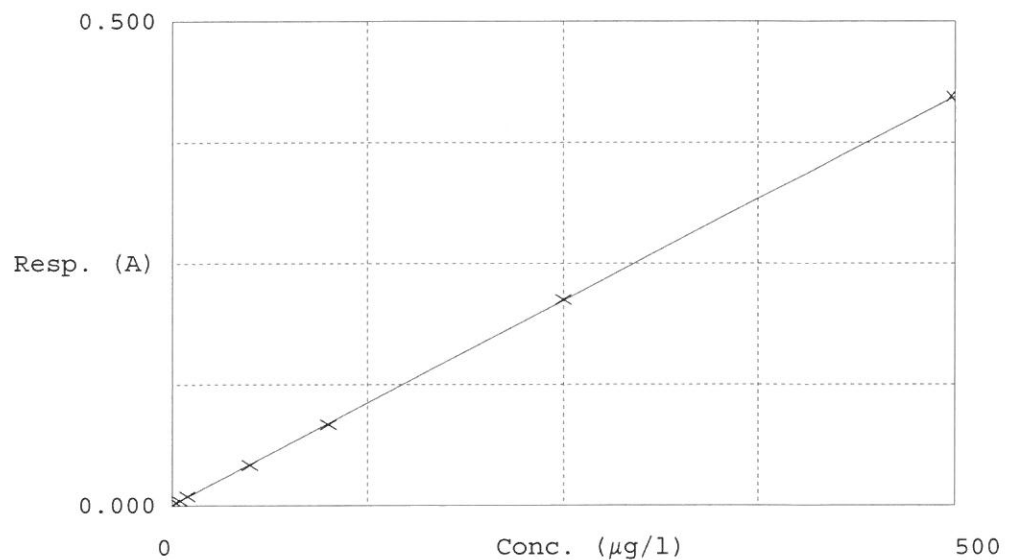

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.8179	0.0000	
2	5.0PPBCN	0.005	5.3286	5.0000	
3	10PPBCN	0.010	10.6226	10.0000	
4	50PPBCN	0.042	48.9125	50.0000	
5	100PPBCN	0.084	98.3458	100.0000	
6	250PPBCN	0.213	251.0975	250.0000	
7	500PPBCN	0.422	499.8751	500.0000	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/26/2019 11:06

Test: Total CN *ug/L*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	92.468	0.0	0.079	
ICB1	1.014	0.0	0.002	
CCV1	238.350	0.0	0.202	
CCB1	1.172	0.0	0.002	
PB123378BL	1.162	0.0	0.002	
PB123378BS	93.508	0.0	0.080	
MIDPB123378	238.549	0.0	0.202	
K4926-02DUP	2.709	0.0	0.003	
K4926-02MSD	37.686	0.0	0.033	
K4926-02MS	40.362	0.0	0.035	
K4926-02	2.522	0.0	0.003	
CCV2	255.953	0.0	0.217	
CCB2	1.192	0.0	0.002	

N	13
Mean	77.434
SD	100.6817
CV%	130.02

9/26/19
CT

Aquakem v. 7.2AQ1

Results from time period:

Thu Sep 26 10:41:23 2019

Thu Sep 26 11:03:49 2019

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.8179	µg/l	9/26/2019 8:17:45	
5.0PPBCN	A	Total CN	P	5.3286	µg/l	9/26/2019 8:17:46	
10PPBCN	A	Total CN	P	10.6226	µg/l	9/26/2019 8:17:47	
50PPBCN	A	Total CN	P	48.9125	µg/l	9/26/2019 8:17:48	
100PPBCN	A	Total CN	P	98.3458	µg/l	9/26/2019 8:17:49	
250PPBCN	A	Total CN	P	251.0975	µg/l	9/26/2019 8:17:50	
500PPBCN	A	Total CN	P	499.8751	µg/l	9/26/2019 8:17:51	
ICV1	S	Total CN	P	92.4685	µg/l	9/26/2019 10:41:23	
ICB1	S	Total CN	P	1.0141	µg/l	9/26/2019 10:41:24	
CCV1	S	Total CN	P	238.3505	µg/l	9/26/2019 10:41:25	
CCB1	S	Total CN	P	1.1723	µg/l	9/26/2019 10:41:26	
PB123378BL	S	Total CN	P	1.1623	µg/l	9/26/2019 10:41:27	
PB123378BS	S	Total CN	P	93.5075	µg/l	9/26/2019 10:41:28	
MIDPB123378	S	Total CN	P	238.5487	µg/l	9/26/2019 10:41:29	
K4926-02DUP	S	Total CN	P	2.7092	µg/l	9/26/2019 10:41:31	
K4926-02MSD	S	Total CN	P	37.6861	µg/l	9/26/2019 10:45:42	
K4926-02MS	S	Total CN	P	40.362	µg/l	9/26/2019 10:45:43	
K4926-02	S	Total CN	P	2.522	µg/l	9/26/2019 11:03:47	
CCV2	S	Total CN	P	255.9534	µg/l	9/26/2019 11:03:48	
CCB2	S	Total CN	P	1.1919	µg/l	9/26/2019 11:03:49	