


LB105331

7471B

INSTRUMENT ID: CV1

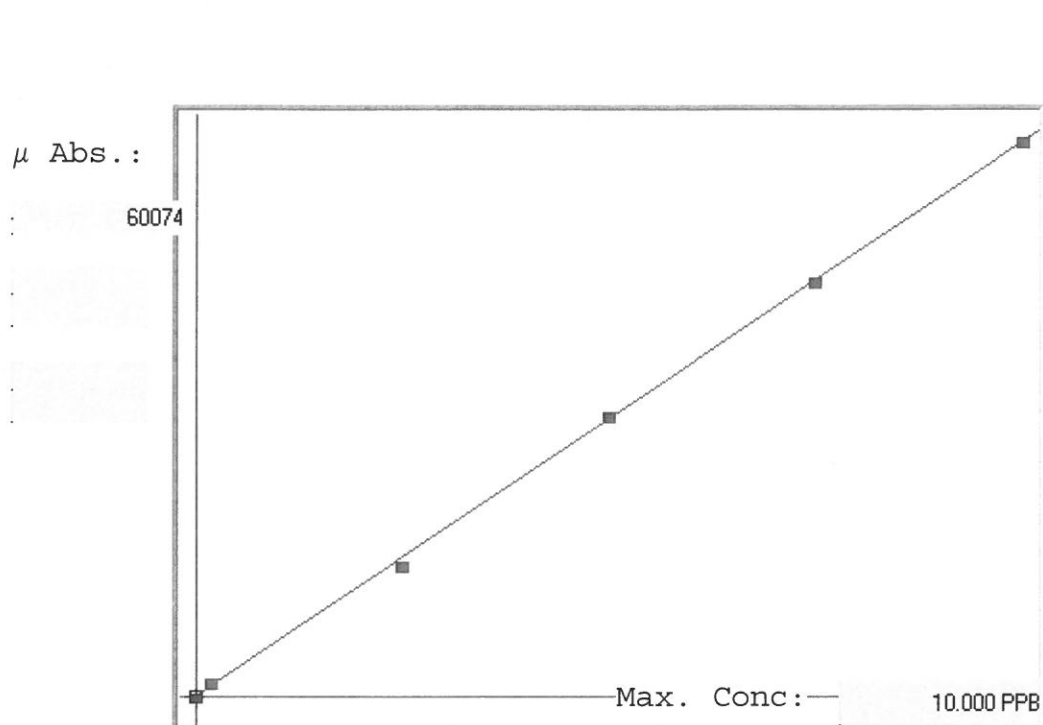

Linear

A= 0.0000e+000

B= 1.6651e-004

C= -3.8687e-003

Rho= 0.9998581

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.011	0.011	87	0.000	87				
0.2	0.200	0.256	0.056	1562	0.0 %	1562				
2.5	2.500	2.374	-0.126	14282	0.0 %	14282				
5.0	5.000	5.064	0.064	30435	0.0 %	30435				
7.5	7.500	7.496	-0.004	45043	0.0 %	45043				
10.0	10.000	9.999	-0.001	60074	0.0 %	60074				

LB105331 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 26 Sep 2019 11:51:04			
Sample ID	Extended ID	µ Abs.	Conc.	Std CondMethod	Units	Date	Type
0.0 - 1	50-0	87	-	0.00007471B	PPB	26 Sep 2019 11:55:01	S Std
0.2 - 1	50-2	1562	-	0.20007471B	PPB	26 Sep 2019 11:57:19	S Std
2.5 - 1	52-5	14282	-	2.50007471B	PPB	26 Sep 2019 11:59:37	S Std
5.0 - 1	55-0	30435	-	5.00007471B	PPB	26 Sep 2019 12:01:55	S Std
7.5 - 1	57-5	45043	-	7.50007471B	PPB	26 Sep 2019 12:04:14	S Std
10.0 - 1	510-0	60074	-	10.00007471B	PPB	26 Sep 2019 12:06:31	S Std
ICV28 - 1	ICV28	24461	4.0691	-7471B	PPB	26 Sep 2019 12:14:02	U SMPL
ICB28 - 1	ICB28	106	0.0138	-7471B	PPB	26 Sep 2019 12:16:18	U SMPL
CCV06 - 1	CCV06	30832	5.1299	-7471B	PPB	26 Sep 2019 12:18:33	U SMPL
CCB06 - 1	CCB06	25	0.0003	-7471B	PPB	26 Sep 2019 12:20:49	U SMPL
CRA - 1	CRA	1548	0.2539	-7471B	PPB	26 Sep 2019 12:23:05	U SMPL
HighStd - 1	HighStd	60648	10.0945	-7471B	PPB	26 Sep 2019 12:25:21	U SMPL
ChkStd - 1	ChkStd	42211	7.0246	-7471B	PPB	26 Sep 2019 12:27:37	U SMPL
PB123408BL - 1	PBS	72	0.0081	-7471B	PPB	26 Sep 2019 12:29:54	U SMPL
PB123408BS - 1	LCSS	22453	3.7347	-7471B	PPB	26 Sep 2019 12:32:10	U SMPL
K4657-01 - 1	BU-02-092419	70632	11.7570	-7471B	PPB	26 Sep 2019 12:34:27	U SMPL
K4657-04 - 1	BU-03-092419	1847	0.3037	-7471B	PPB	26 Sep 2019 12:36:44	U SMPL
K4663-07 - 1	OK-02-092419	5850	0.9702	-7471B	PPB	26 Sep 2019 12:39:03	U SMPL
K4663-07DUP - 1	OK-02-092419DUP	5845	0.9694	-7471B	PPB	26 Sep 2019 12:41:21	U SMPL
K4663-07MS - 1	OK-02-092419MS	28867	4.8027	-7471B	PPB	26 Sep 2019 12:43:36	U SMPL
CCV07 - 1	CCV07	31022	5.1616	-7471B	PPB	26 Sep 2019 12:45:52	U SMPL
CCB07 - 1	CCB07	23	-0.0000	-7471B	PPB	26 Sep 2019 12:48:08	U SMPL
K4663-07MSD - 1	OK-02-092419MSD	24166	4.0200	-7471B	PPB	26 Sep 2019 12:50:24	U SMPL
K4822-03 - 1	SB-3A-(15-16)	364	0.0567	-7471B	PPB	26 Sep 2019 12:52:40	U SMPL
K4822-12 - 1	SB-3B-(15-16)	2386	0.3934	-7471B	PPB	26 Sep 2019 12:54:56	U SMPL
K5020-01 - 1	RT-3860	3207	0.5301	-7471B	PPB	26 Sep 2019 12:57:13	U SMPL
K5020-03 - 1	RT-3465	2830	0.4674	-7471B	PPB	26 Sep 2019 12:59:30	U SMPL
K5020-05 - 1	RT-5124	951	0.1545	-7471B	PPB	26 Sep 2019 13:01:46	U SMPL
K5020-07 - 1	RBR-200050	1180	0.1926	-7471B	PPB	26 Sep 2019 13:04:04	U SMPL
K5021-01 - 1	RT-1488-RBR200031-RBR200036	5829	0.9667	-7471B	PPB	26 Sep 2019 13:06:21	U SMPL
K4663-07LX5 - 1		1261	0.2061	-7471B	PPB	26 Sep 2019 13:08:39	U SMPL
K4663-07A - 1		26705	4.4427	-7471B	PPB	26 Sep 2019 13:10:55	U SMPL
CCV08 - 1	CCV08	31263	5.2017	-7471B	PPB	26 Sep 2019 13:13:12	U SMPL
CCB08 - 1	CCB08	38	0.0025	-7471B	PPB	26 Sep 2019 13:15:27	U SMPL
K4657-01DLX2 - 1		35883	5.9710	-7471B	PPB	26 Sep 2019 13:17:44	U SMPL
CCV09 - 1	CCV09	30913	5.1434	-7471B	PPB	26 Sep 2019 13:20:00	U SMPL
CCB09 - 1	CCB09	109	0.0143	-7471B	PPB	26 Sep 2019 13:22:16	U SMPL