


LB105341

245.1

INSTRUMENT ID : CV1

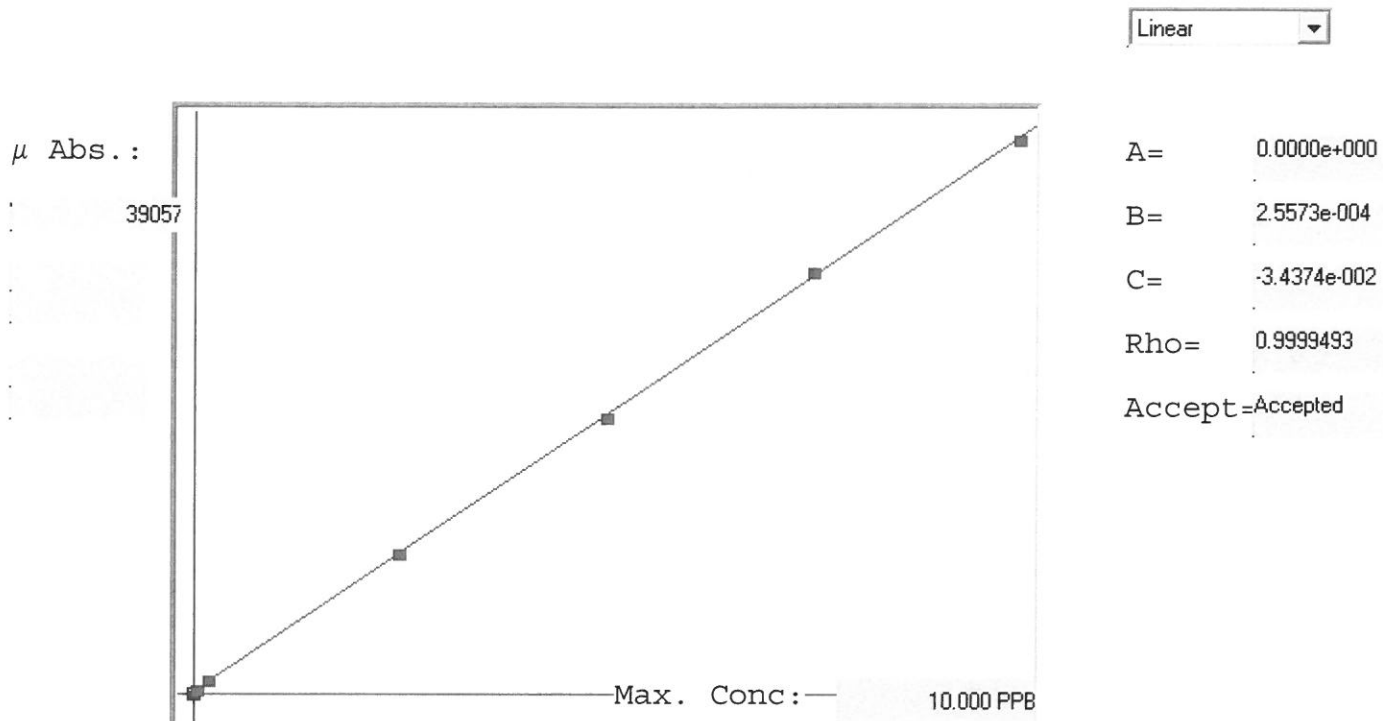

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.014	-0.014	79	0.000	79				
0.05	0.050	0.039	-0.011	286	0.0 %	286				
0.2	0.200	0.223	0.023	1007	0.0 %	1007				
2.5	2.500	2.496	-0.004	9893	0.0 %	9893				
5.0	5.000	4.975	-0.025	19588	0.0 %	19588				
7.5	7.500	7.578	0.078	29768	0.0 %	29768				
10.0	10.000	9.954	-0.046	39057	0.0 %	39057				

LB105341 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 26 Sep 2019 14:28:07

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	79	-	0.0000	245.1	PPB	26 Sep 2019 14:33:31	S	Std
0.05 - 1	50.05	286	-	0.0500	245.1	PPB	26 Sep 2019 14:35:49	S	Std
0.2 - 1	50.2	1007	-	0.2000	245.1	PPB	26 Sep 2019 14:38:08	S	Std
2.5 - 1	52.5	9893	-	2.5000	245.1	PPB	26 Sep 2019 14:42:17	S	Std
5.0 - 1	55.0	19588	-	5.0000	245.1	PPB	26 Sep 2019 14:44:35	S	Std
7.5 - 1	57.5	29768	-	7.5000	245.1	PPB	26 Sep 2019 14:46:52	S	Std
10.0 - 1	510.0	39057	-	10.0000	245.1	PPB	26 Sep 2019 14:57:13	S	Std
ICV29 - 1	ICV29	15285	3.8745	-245.1		PPB	26 Sep 2019 15:00:27	U	SMPL
ICB29 - 1	ICB29	-39	-0.0443	-245.1		PPB	26 Sep 2019 15:02:43	U	SMPL
CCV10 - 1	CCV10	19376	4.9206	-245.1		PPB	26 Sep 2019 15:04:59	U	SMPL
CCB10 - 1	CCB10	-24	-0.0405	-245.1		PPB	26 Sep 2019 15:07:15	U	SMPL
CRA - 1	CRA	314	0.0459	-245.1		PPB	26 Sep 2019 15:09:31	U	SMPL
HighStd - 1	HighStd	38499	9.8110	-245.1		PPB	26 Sep 2019 15:11:46	U	SMPL
ChkStd - 1	ChkStd	27048	6.8826	-245.1		PPB	26 Sep 2019 15:14:02	U	SMPL
PB123416BL - 1	PBW	-72	-0.0528	-245.1		PPB	26 Sep 2019 15:16:21	U	SMPL
PB123416BS - 1	LCSW	15553	3.9430	-245.1		PPB	26 Sep 2019 15:18:39	U	SMPL
K4788-02 - 1	FALL-2019	444	0.0792	-245.1		PPB	26 Sep 2019 15:20:55	U	SMPL
K4788-02DUP - 1	FALL-2019DUP	398	0.0674	-245.1		PPB	26 Sep 2019 15:23:13	U	SMPL
K4788-02MS - 1	FALL-2019MS	13856	3.5090	-245.1		PPB	26 Sep 2019 15:25:31	U	SMPL
K4788-02MSD - 1	FALL-2019MSD	14161	3.5870	-245.1		PPB	26 Sep 2019 15:27:49	U	SMPL
K4926-01 - 1	EFFLUENT-DAY1-METALS	121	-0.0034	-245.1		PPB	26 Sep 2019 15:30:07	U	SMPL
CCV11 - 1	CCV11	19403	4.9275	-245.1		PPB	26 Sep 2019 15:32:24	U	SMPL
CCB11 - 1	CCB11	-7	-0.0362	-245.1		PPB	26 Sep 2019 15:34:39	U	SMPL
PB123417BL - 1	PBW	-20	-0.0395	-245.1		PPB	26 Sep 2019 15:36:55	U	SMPL
PB123417BS - 1	LCSW	15472	3.9223	-245.1		PPB	26 Sep 2019 15:39:11	U	SMPL
K4841-08 - 1	PT-HG-WP	29141	7.4178	-245.1		PPB	26 Sep 2019 15:41:27	U	SMPL
K4788-02LX5 - 1		141	0.0017	-245.1		PPB	26 Sep 2019 15:46:01	U	SMPL
K4788-02A - 1		14212	3.6001	-245.1		PPB	26 Sep 2019 15:48:19	U	SMPL
CCV12 - 1	CCV12	19387	4.9235	-245.1		PPB	26 Sep 2019 15:50:35	U	SMPL
CCB12 - 1	CCB12	-59	-0.0495	-245.1		PPB	26 Sep 2019 15:52:54	U	SMPL