


LB105349

7471B

INSTRUMENT ID: C U 1

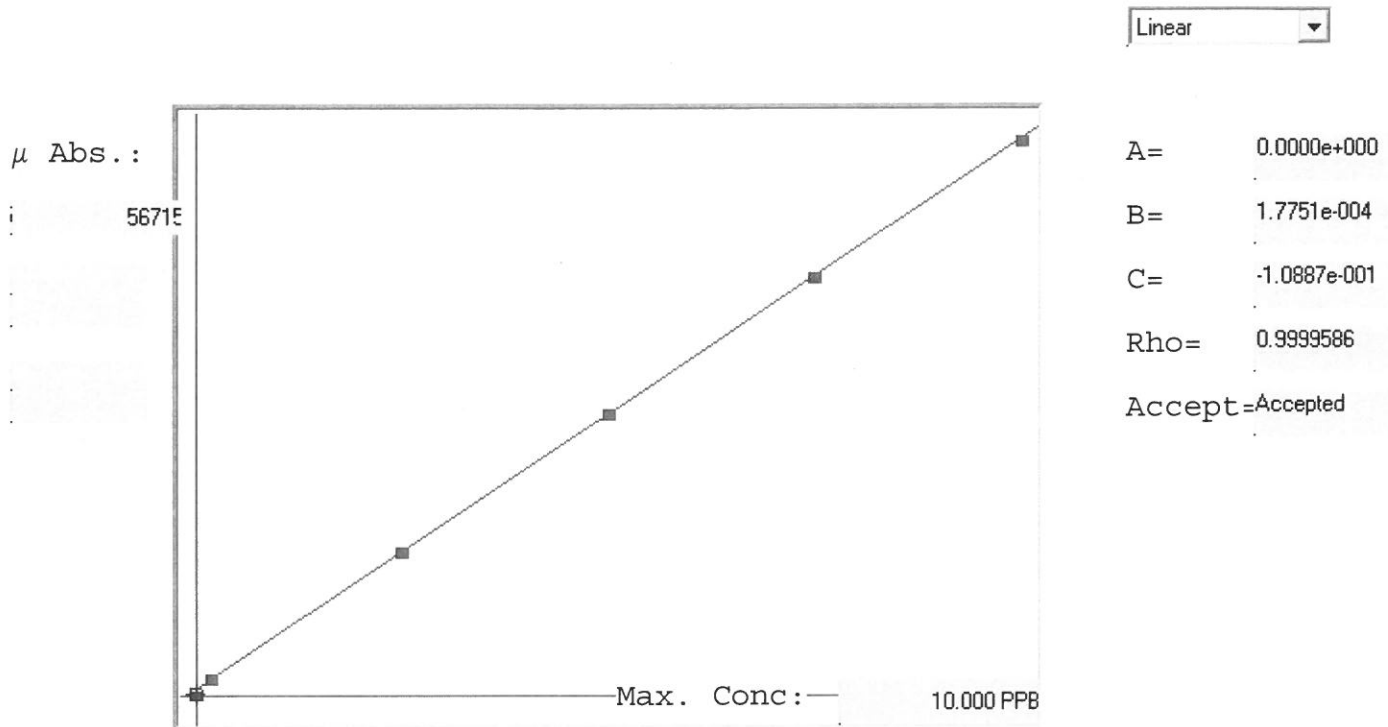

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.048	-0.048	344	0.000	344				
0.2	0.200	0.210	0.010	1795	0.0 %	1795				
2.5	2.500	2.515	0.015	14782	0.0 %	14782				
5.0	5.000	5.046	0.046	29040	0.0 %	29040				
7.5	7.500	7.518	0.018	42966	0.0 %	42966				
10.0	10.000	9.959	-0.041	56715	0.0 %	56715				

LB105349 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 27 Sep 2019 09:36:51					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	344	-	0.0000	7471B	PPB	27 Sep 2019 09:36:59	S	Std
0.2 - 1	50.2	1795	-	0.2000	7471B	PPB	27 Sep 2019 09:39:17	S	Std
2.5 - 1	52.5	14782	-	2.5000	7471B	PPB	27 Sep 2019 09:41:35	S	Std
5.0 - 1	55.0	29040	-	5.0000	7471B	PPB	27 Sep 2019 09:43:53	S	Std
7.5 - 1	57.5	42966	-	7.5000	7471B	PPB	27 Sep 2019 09:46:11	S	Std
10.0 - 1	510.0	56715	-	10.0000	7471B	PPB	27 Sep 2019 09:48:28	S	Std
ICV30 - 1	ICV30	23354	4.0367	-	7471B	PPB	27 Sep 2019 09:51:13	U	SMPL
ICB30 - 1	ICB30	328	-0.0506	-	7471B	PPB	27 Sep 2019 09:53:28	U	SMPL
CCV13 - 1	CCV13	29380	5.1064	-	7471B	PPB	27 Sep 2019 09:55:44	U	SMPL
CCB13 - 1	CCB13	334	-0.0496	-	7471B	PPB	27 Sep 2019 09:58:00	U	SMPL
CRA - 1	CRA	1819	0.2140	-	7471B	PPB	27 Sep 2019 10:00:17	U	SMPL
HighStd - 1	HighStd	57622	10.1197	-	7471B	PPB	27 Sep 2019 10:02:33	U	SMPL
ChkStd - 1	ChkStd	39624	6.9249	-	7471B	PPB	27 Sep 2019 10:04:50	U	SMPL
PB123430BL - 1	PBS	-32	-0.1145	-	7471B	PPB	27 Sep 2019 10:07:07	U	SMPL
PB123430BS - 1	LCSS	21020	3.6224	-	7471B	PPB	27 Sep 2019 10:09:25	U	SMPL
K4668-16 - 1	SU-04-092619	1601	0.1753	-	7471B	PPB	27 Sep 2019 10:11:42	U	SMPL
K5038-01 - 1	DN-1	17624	3.0196	-	7471B	PPB	27 Sep 2019 10:14:00	U	SMPL
K5038-03 - 1	DN-2	46960	8.2271	-	7471B	PPB	27 Sep 2019 10:16:17	U	SMPL
K5038-05 - 1	DN-3	23235	4.0156	-	7471B	PPB	27 Sep 2019 10:18:34	U	SMPL
K5038-05DUP - 1	DN-3DUP	23334	4.0332	-	7471B	PPB	27 Sep 2019 10:20:51	U	SMPL
CCV14 - 1	CCV14	29124	5.0610	-	7471B	PPB	27 Sep 2019 10:23:07	U	SMPL
CCB14 - 1	CCB14	284	-0.0585	-	7471B	PPB	27 Sep 2019 10:25:24	U	SMPL
K5038-05MS - 1	DN-3MS	46014	8.0592	-	7471B	PPB	27 Sep 2019 10:27:40	U	SMPL
K5038-05MSD - 1	DN-3MSD	43965	7.6954	-	7471B	PPB	27 Sep 2019 10:29:56	U	SMPL
K5038-07 - 1	TS-1	38352	6.6991	-	7471B	PPB	27 Sep 2019 10:32:14	U	SMPL
K5038-09 - 1	TS-2	24410	4.2242	-	7471B	PPB	27 Sep 2019 10:34:30	U	SMPL
K5038-11 - 1	TS-3	28940	5.0283	-	7471B	PPB	27 Sep 2019 10:36:47	U	SMPL
K5060-01 - 1	FK-PS-01-060	3386	0.4922	-	7471B	PPB	27 Sep 2019 10:39:04	U	SMPL
K5038-05LX5 - 1		4754	0.7350	-	7471B	PPB	27 Sep 2019 10:44:27	U	SMPL
K5038-05A - 1		44659	7.8186	-	7471B	PPB	27 Sep 2019 10:46:44	U	SMPL
CCV15 - 1	CCV15	29279	5.0885	-	7471B	PPB	27 Sep 2019 10:49:02	U	SMPL
CCB15 - 1	CCB15	284	-0.0585	-	7471B	PPB	27 Sep 2019 10:51:19	U	SMPL