


LB105381

7470A

INSTRUMENT ID : CU1

Linear

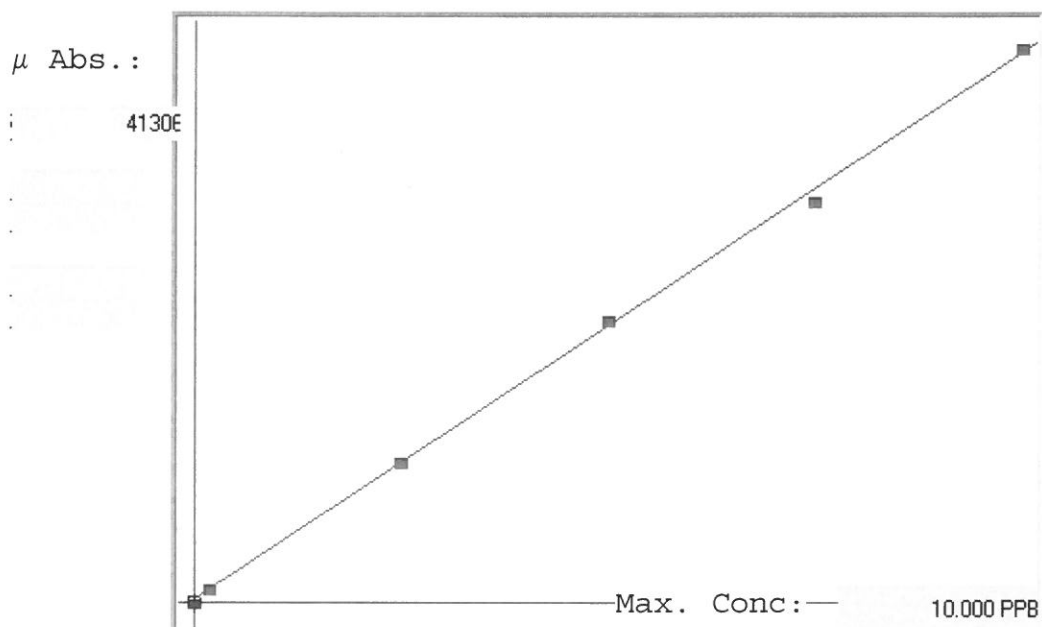

A= 0.0000e+000

B= 2.4515e-004

C= -4.9895e-002

Rho= 0.9996443

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.015	-0.015	141	0.000	141				
0.2	0.200	0.196	-0.004	1001	0.0 %	1001				
2.5	2.500	2.521	0.021	10486	0.0 %	10486				
5.0	5.000	5.117	0.117	21077	0.0 %	21077				
7.5	7.500	7.305	-0.195	30003	0.0 %	30003				
10.0	10.000	10.076	0.076	41306	0.0 %	41306				

LB105381 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 30 Sep 2019 12:40:09

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	141	-	0.0000	7470A	PPB	30 Sep 2019 12:44:18	S	Std
0.2 - 1	50.2	1001	-	0.2000	7470A	PPB	30 Sep 2019 12:46:27	S	Std
2.5 - 1	52.5	10486	-	2.5000	7470A	PPB	30 Sep 2019 12:48:37	S	Std
5.0 - 1	55.0	21077	-	5.0000	7470A	PPB	30 Sep 2019 12:50:45	S	Std
7.5 - 1	57.5	30003	-	7.5000	7470A	PPB	30 Sep 2019 12:52:54	S	Std
10.0 - 1	510.0	41306	-	10.0000	7470A	PPB	30 Sep 2019 12:55:01	S	Std
ICV33 - 1	ICV33	17036	4.1265	-	7470A	PPB	30 Sep 2019 12:57:38	U	SMPL
ICB33 - 1	ICB33	108	-0.0234	-	7470A	PPB	30 Sep 2019 12:59:44	U	SMPL
CCV27 - 1	CCV27	21122	5.1282	-	7470A	PPB	30 Sep 2019 13:01:51	U	SMPL
CCB27 - 1	CCB27	100	-0.0254	-	7470A	PPB	30 Sep 2019 13:03:57	U	SMPL
CRA - 1	CRA	1017	0.1994	-	7470A	PPB	30 Sep 2019 13:06:04	U	SMPL
HighStd - 1	HighStd	40784	9.9484	-	7470A	PPB	30 Sep 2019 13:08:11	U	SMPL
ChkStd - 1	ChkStd	28365	6.9039	-	7470A	PPB	30 Sep 2019 13:10:17	U	SMPL
PB123499BL - 1	PBW	74	-0.0318	-	7470A	PPB	30 Sep 2019 13:12:25	U	SMPL
PB123499BS - 1	LCSW	16187	3.9184	-	7470A	PPB	30 Sep 2019 13:14:32	U	SMPL
K5088-01 - 1	SP-NATURAL-GAS-HEATER	152	-0.0126	-	7470A	PPB	30 Sep 2019 13:16:41	U	SMPL
K5088-01DUP - 1	SP-NATURAL-GAS-HEATERDUP	166	-0.0092	-	7470A	PPB	30 Sep 2019 13:18:49	U	SMPL
K5088-01MS - 1	SP-NATURAL-GAS-HEATERMS	16379	3.9655	-	7470A	PPB	30 Sep 2019 13:23:58	U	SMPL
K5088-01MSD - 1	SP-NATURAL-GAS-HEATERMSD	15660	3.7892	-	7470A	PPB	30 Sep 2019 13:26:08	U	SMPL
K5088-01LX5 - 1		92	-0.0273	-	7470A	PPB	30 Sep 2019 13:28:16	U	SMPL
CCV28 - 1	CCV28	21123	5.1285	-	7470A	PPB	30 Sep 2019 13:30:23	U	SMPL
CCB28 - 1	CCB28	106	-0.0239	-	7470A	PPB	30 Sep 2019 13:32:31	U	SMPL
K5088-01A - 1		15990	3.8701	-	7470A	PPB	30 Sep 2019 13:34:40	U	SMPL
CCV29 - 1	CCV29	21102	5.1233	-	7470A	PPB	30 Sep 2019 13:36:46	U	SMPL
CCB29 - 1	CCB29	48	-0.0381	-	7470A	PPB	30 Sep 2019 13:38:54	U	SMPL