


LB105397

7470A

INSTRUMENT ID : CU1

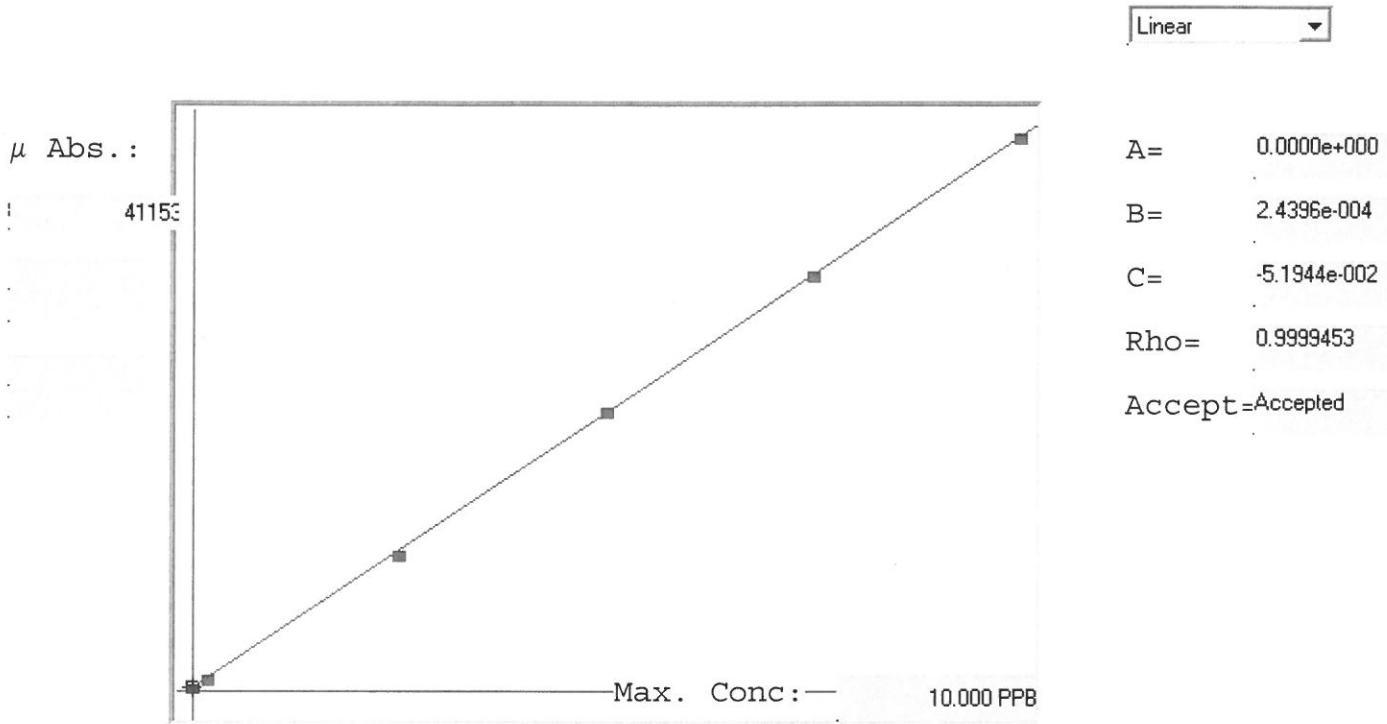

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.042	0.042	384	0.000	384				
0.2	0.200	0.183	-0.017	965	0.0 %	965				
2.5	2.500	2.433	-0.067	10187	0.0 %	10187				
5.0	5.000	5.048	0.048	20904	0.0 %	20904				
7.5	7.500	7.506	0.006	30980	0.0 %	30980				
10.0	10.000	9.988	-0.012	41153	0.0 %	41153				

LB105397 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 01 Oct 2019 09:34:46

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	S8.0	384	-	0.0000	7470A	PPB	01 Oct 2019 09:47:22	S	Std
0.2 - 1	S8.2	965	-	0.2000	7470A	PPB	01 Oct 2019 09:49:32	S	Std
2.5 - 1	S2.5	10187	-	2.5000	7470A	PPB	01 Oct 2019 09:51:41	S	Std
5.0 - 1	S5.0	20904	-	5.0000	7470A	PPB	01 Oct 2019 09:53:49	S	Std
7.5 - 1	S7.5	30980	-	7.5000	7470A	PPB	01 Oct 2019 09:55:58	S	Std
10.0 - 1	S10.0	41153	-	10.0000	7470A	PPB	01 Oct 2019 09:58:06	S	Std
ICV34 - 1	ICV34	16327	3.9312	-	7470A	PPB	01 Oct 2019 10:00:37	U	SMPL
ICB34 - 1	ICB34	181	-0.0078	-	7470A	PPB	01 Oct 2019 10:02:44	U	SMPL
CCV30 - 1	CCV30	20885	5.0432	-	7470A	PPB	01 Oct 2019 10:04:51	U	SMPL
CCB30 - 1	CCB30	206	-0.0017	-	7470A	PPB	01 Oct 2019 10:08:41	U	SMPL
CRA - 1	CRA	964	0.1832	-	7470A	PPB	01 Oct 2019 10:10:48	U	SMPL
HighStd - 1	HighStd	40884	9.9221	-	7470A	PPB	01 Oct 2019 10:12:55	U	SMPL
ChkStd - 1	ChkStd	28795	6.9729	-	7470A	PPB	01 Oct 2019 10:15:02	U	SMPL
PB123519BL - 1	PBW	146	-0.0163	-	7470A	PPB	01 Oct 2019 10:17:09	U	SMPL
PB123519BS - 1	LCSW	16651	4.0102	-	7470A	PPB	01 Oct 2019 10:19:17	U	SMPL
K4668-19 - 1	SU-04-092619	114	-0.0241	-	7470A	PPB	01 Oct 2019 10:21:24	U	SMPL
K4668-19DUP - 1	SU-04-092619DUP	138	-0.0183	-	7470A	PPB	01 Oct 2019 10:25:11	U	SMPL
K4668-19MS - 1	SU-04-092619MS	17137	4.1288	-	7470A	PPB	01 Oct 2019 10:27:19	U	SMPL
K4668-19MSD - 1	SU-04-092619MSD	17195	4.1430	-	7470A	PPB	01 Oct 2019 10:29:28	U	SMPL
K5079-04 - 1	TP-1-COMP	1011	0.1947	-	7470A	PPB	01 Oct 2019 10:31:35	U	SMPL
CCV31 - 1	CCV31	20855	5.0358	-	7470A	PPB	01 Oct 2019 10:33:42	U	SMPL
CCB31 - 1	CCB31	111	-0.0249	-	7470A	PPB	01 Oct 2019 10:35:49	U	SMPL
K5093-07 - 1	SB-01-COMP	551	0.0825	-	7470A	PPB	01 Oct 2019 10:37:56	U	SMPL
K5093-08 - 1	SB-02-COMP	422	0.0510	-	7470A	PPB	01 Oct 2019 10:40:03	U	SMPL
K5093-09 - 1	SB-03-COMP	345	0.0322	-	7470A	PPB	01 Oct 2019 10:42:10	U	SMPL
K5094-06 - 1	MC-17-COMPOSITE	288	0.0183	-	7470A	PPB	01 Oct 2019 10:44:17	U	SMPL
PB123520BL - 1	PBW	218	0.0012	-	7470A	PPB	01 Oct 2019 10:46:24	U	SMPL
PB123520BS - 1	LCSW	17147	4.1312	-	7470A	PPB	01 Oct 2019 10:49:24	U	SMPL
K5095-04 - 1	COMPOSITE-4	12532	3.0054	-	7470A	PPB	01 Oct 2019 10:51:31	U	SMPL
K5095-04DUP - 1	COMPOSITE-4DUP	13079	3.1388	-	7470A	PPB	01 Oct 2019 10:53:40	U	SMPL
K5095-04MS - 1	COMPOSITE-4MS	28286	6.8487	-	7470A	PPB	01 Oct 2019 10:59:41	U	SMPL
K5095-04MSD - 1	COMPOSITE-4MSD	27783	6.7260	-	7470A	PPB	01 Oct 2019 11:01:48	U	SMPL
CCV32 - 1	CCV32	20964	5.0624	-	7470A	PPB	01 Oct 2019 11:03:56	U	SMPL
CCB32 - 1	CCB32	132	-0.0197	-	7470A	PPB	01 Oct 2019 11:06:05	U	SMPL
K5095-05 - 1	COMPOSITE-5	22213	5.3671	-	7470A	PPB	01 Oct 2019 11:08:12	U	SMPL
PB123519TB - 1	PB123436TB	253	0.0098	-	7470A	PPB	01 Oct 2019 11:10:19	U	SMPL
K4668-19LX5 - 1		17	-0.0478	-	7470A	PPB	01 Oct 2019 11:12:27	U	SMPL
K4668-19A - 1		17191	4.1420	-	7470A	PPB	01 Oct 2019 11:14:34	U	SMPL
K5095-04LX5 - 1		2482	0.5536	-	7470A	PPB	01 Oct 2019 11:16:41	U	SMPL
K5095-04A - 1		27797	6.7294	-	7470A	PPB	01 Oct 2019 11:18:49	U	SMPL
CCV33 - 1	CCV33	21042	5.0815	-	7470A	PPB	01 Oct 2019 11:23:07	U	SMPL
CCB33 - 1	CCB33	162	-0.0124	-	7470A	PPB	01 Oct 2019 11:25:16	U	SMPL