


LB105408

245.1

INSTRUMENT ID : CV1

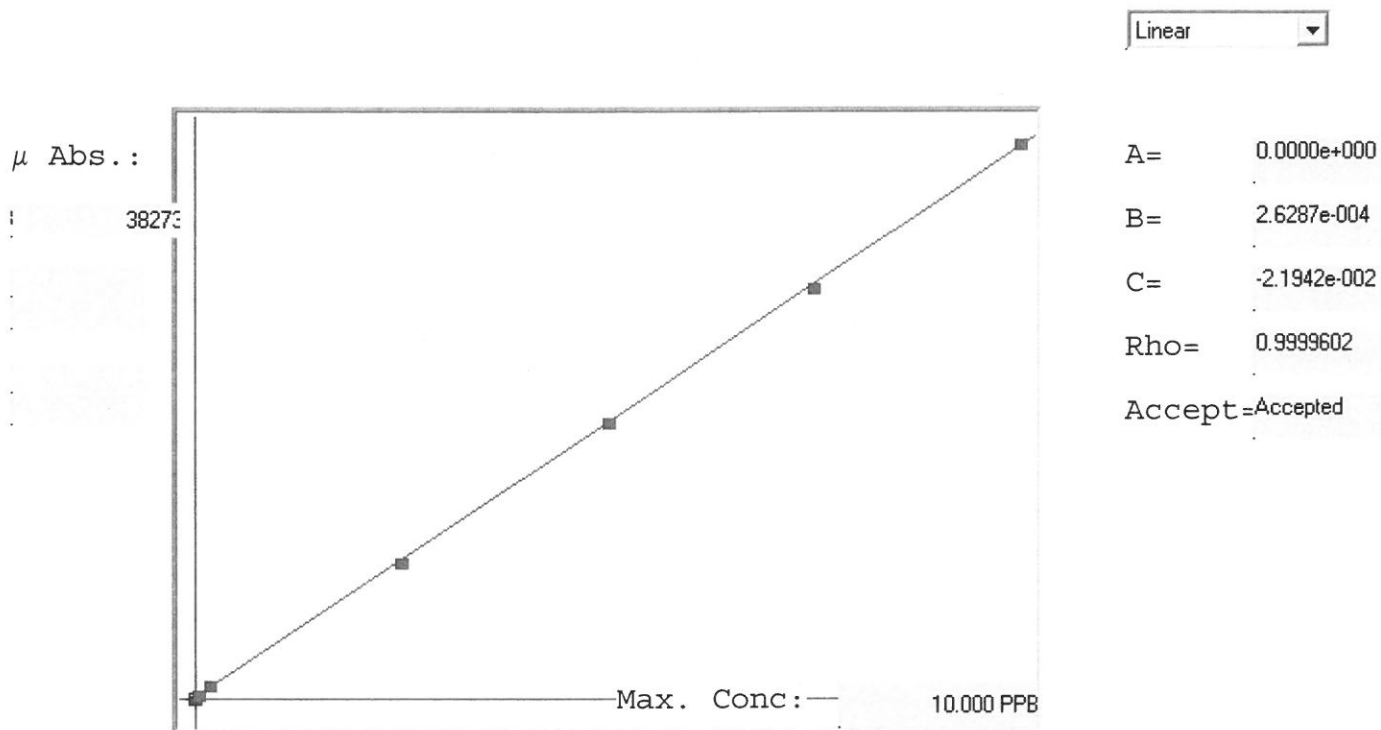

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.006	0.006	108	0.000	108				
0.05	0.050	0.056	0.006	298	0.0 %	298				
0.2	0.200	0.228	0.028	951	0.0 %	951				
2.5	2.500	2.451	-0.049	9408	0.0 %	9408				
5.0	5.000	5.019	0.019	19178	0.0 %	19178				
7.5	7.500	7.450	-0.050	28423	0.0 %	28423				
10.0	10.000	10.039	0.039	38273	0.0 %	38273				

LB105408 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 01 Oct 2019 15:03:37

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	108	-	0.0000	245.1	PPB	01 Oct 2019 15:16:48	S	Std
0.05 - 1	50.05	298	-	0.0500	245.1	PPB	01 Oct 2019 15:19:06	S	Std
0.2 - 1	50.2	951	-	0.2000	245.1	PPB	01 Oct 2019 15:21:24	S	Std
2.5 - 1	52.5	9408	-	2.5000	245.1	PPB	01 Oct 2019 15:23:42	S	Std
5.0 - 1	55.0	19178	-	5.0000	245.1	PPB	01 Oct 2019 15:26:00	S	Std
7.5 - 1	57.5	28423	-	7.5000	245.1	PPB	01 Oct 2019 15:28:16	S	Std
10.0 - 1	510.0	38273	-	10.0000	245.1	PPB	01 Oct 2019 15:39:27	S	Std
ICV36 - 1	ICV36	14878	3.8891	-245.1		PPB	01 Oct 2019 15:44:55	U	SMPL
ICB36 - 1	ICB36	7	-0.0201	-245.1		PPB	01 Oct 2019 15:47:10	U	SMPL
CCV39 - 1	CCV39	18888	4.9432	-245.1		PPB	01 Oct 2019 15:49:26	U	SMPL
CCB39 - 1	CCB39	23	-0.0159	-245.1		PPB	01 Oct 2019 15:51:42	U	SMPL
CRA - 1	CRA	249	0.0435	-245.1		PPB	01 Oct 2019 15:53:58	U	SMPL
HighStd - 1	HighStd	38273	10.0389	-245.1		PPB	01 Oct 2019 15:56:14	U	SMPL
ChkStd - 1	ChkStd	25848	6.7727	-245.1		PPB	01 Oct 2019 15:58:30	U	SMPL
PB123546BL - 1	PBW	-8	-0.0240	-245.1		PPB	01 Oct 2019 16:00:48	U	SMPL
PB123546BS - 1	LCSW	15257	3.9887	-245.1		PPB	01 Oct 2019 16:03:05	U	SMPL
K5111-10 - 1	LOD-MDL-WATER-04-QT4-2019	238	0.0406	-245.1		PPB	01 Oct 2019 16:05:22	U	SMPL
K5111-11 - 1	LOQ-WATER-05-QT4-2019	1503	0.3732	-245.1		PPB	01 Oct 2019 16:07:39	U	SMPL
PB123547BL - 1	PBW	0	-0.0219	-245.1		PPB	01 Oct 2019 16:09:57	U	SMPL
PB123547BS - 1	LCSW	17330	4.5336	-245.1		PPB	01 Oct 2019 16:12:15	U	SMPL
K4973-02 - 1	EFF-WW	103	0.0051	-245.1		PPB	01 Oct 2019 16:14:31	U	SMPL
CCV40 - 1	CCV40	18953	4.9603	-245.1		PPB	01 Oct 2019 16:16:47	U	SMPL
CCB40 - 1	CCB40	-31	-0.0301	-245.1		PPB	01 Oct 2019 16:19:03	U	SMPL
K4973-02DUP - 1	EFF-WWDUP	222	0.0364	-245.1		PPB	01 Oct 2019 16:21:19	U	SMPL
K4973-02MS - 1	EFF-WWMS	14007	3.6601	-245.1		PPB	01 Oct 2019 16:23:35	U	SMPL
K4973-02MSD - 1	EFF-WWMSD	12365	3.2285	-245.1		PPB	01 Oct 2019 16:25:51	U	SMPL
K4973-02LX5 - 1		10	-0.0193	-245.1		PPB	01 Oct 2019 16:28:08	U	SMPL
K4973-02A - 1		13125	3.4282	-245.1		PPB	01 Oct 2019 16:30:26	U	SMPL
CCV41 - 1	CCV41	19084	4.9947	-245.1		PPB	01 Oct 2019 16:32:43	U	SMPL
CCB41 - 1	CCB41	2	-0.0214	-245.1		PPB	01 Oct 2019 16:35:01	U	SMPL