

LB105599

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

10/9/2019 16:05


Test Phenolics-

Accepted 10/9/2019 16:05

Factor 9.015
Bias 0.013

Coeff. of det. 0.999878

Errors

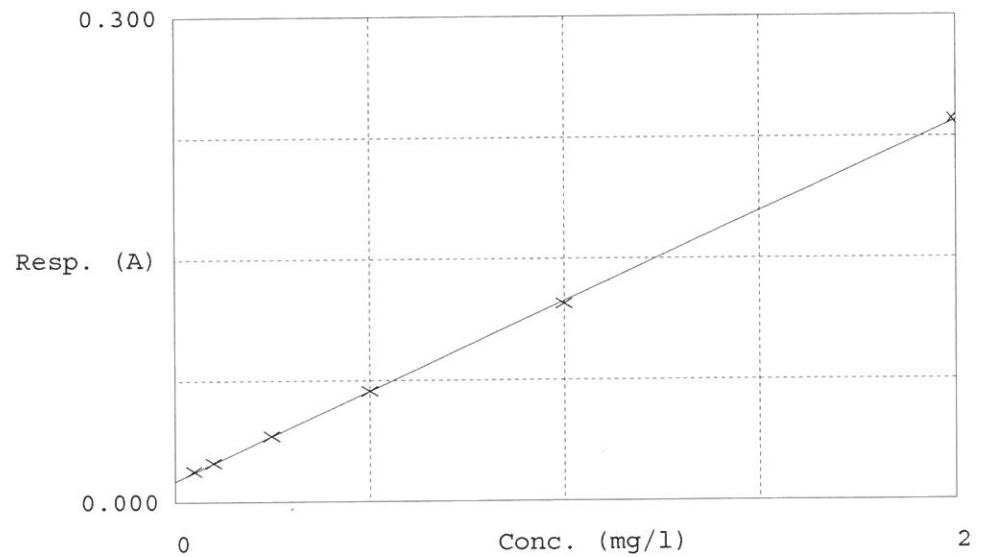

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.019	0.0559	0.0500	
2	Phenol-2	0.024	0.1015	0.1000	
3	Phenol-2	0.041	0.2508	0.2500	
4	Phenol-2	0.069	0.5000	0.5000	
5	Phenol-2	0.122	0.9843	1.0000	
6	Phenol-2	0.236	2.0075	2.0000	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

10/9/2019 16:52

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.006	0.0	0.125	
ICB1	-0.008	0.0	0.012	
CCV1	1.007	0.0	0.125	
CCB1	0.000	0.0	0.013	
PB123759BL	-0.009	0.0	0.012	
PB123759BS	0.998	0.0	0.124	
K5111-07	0.008	0.0	0.014	
K5111-08	0.045	0.0	0.018	
PB123757BL	0.001	0.0	0.013	
PB123757BS	1.017	0.0	0.126	
K5111-01	0.009	0.0	0.014	
K5111-02	0.040	0.0	0.017	
CCV2	1.047	0.0	0.129	
CCB2	0.025	0.0	0.016	

N	14
Mean	0.370
SD	0.4990
CV%	134.71

10/9/19

CT

Aquakem v. 7.2AQ1

Results from time period:

Wed Oct 09 15:32:56 2019

Wed Oct 09 16:48:21 2019

Sample Id	Sam/Ctr/c	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0559	mg/l	10/9/2019 15:32:56	
0.1PPM	A	Phenolics-	P	0.1015	mg/l	10/9/2019 15:32:57	
0.25PPM	A	Phenolics-	P	0.2508	mg/l	10/9/2019 15:32:58	
0.50PPM	A	Phenolics-	P	0.5	mg/l	10/9/2019 15:32:59	
1.0PPM	A	Phenolics-	P	0.9843	mg/l	10/9/2019 15:33:00	
2.0PPM	A	Phenolics-	P	2.0075	mg/l	10/9/2019 15:33:01	
ICV1	S	Phenolics-	P	1.0062	mg/l	10/9/2019 16:22:45	
ICB1	S	Phenolics-	P	-0.0078	mg/l	10/9/2019 16:22:46	
CCV1	S	Phenolics-	P	1.007	mg/l	10/9/2019 16:22:47	
CCB1	S	Phenolics-	P	0.0005	mg/l	10/9/2019 16:22:48	
PB123759BL	S	Phenolics-	P	-0.0091	mg/l	10/9/2019 16:22:49	
PB123759BS	S	Phenolics-	P	0.9978	mg/l	10/9/2019 16:22:50	
K5111-07	S	Phenolics-	P	0.0084	mg/l	10/9/2019 16:22:51	
K5111-08	S	Phenolics-	P	0.0448	mg/l	10/9/2019 16:22:52	
PB123757BL	S	Phenolics-	P	0.001	mg/l	10/9/2019 16:22:53	
PB123757BS	S	Phenolics-	P	1.0171	mg/l	10/9/2019 16:22:54	
K5111-01	S	Phenolics-	P	0.0087	mg/l	10/9/2019 16:27:39	
K5111-02	S	Phenolics-	P	0.0395	mg/l	10/9/2019 16:27:41	
CCV2	S	Phenolics-	P	1.0473	mg/l	10/9/2019 16:48:20	
CCB2	S	Phenolics-	P	0.0246	mg/l	10/9/2019 16:48:21	