


LB105605

7471B

INSTRUMENT ID: CV1

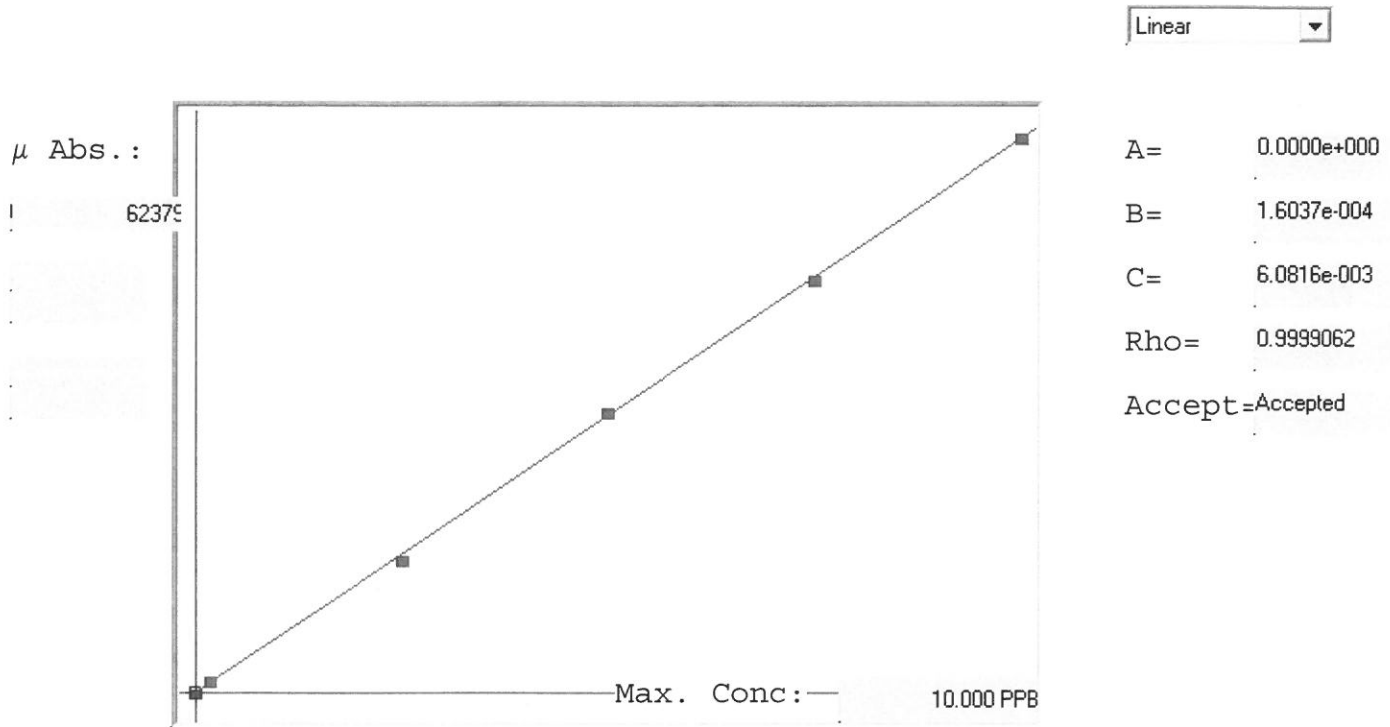

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.019	0.019	80	0.000	80				
0.2	0.200	0.232	0.032	1406	0.0 %	1406				
2.5	2.500	2.403	-0.097	14944	0.0 %	14944				
5.0	5.000	5.062	0.062	31525	0.0 %	31525				
7.5	7.500	7.476	-0.024	46578	0.0 %	46578				
10.0	10.000	10.010	0.010	62379	0.0 %	62379				

LB105605 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 10 Oct 2019 08:46:57

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50.0	80	-	0.00007471B	PPB	10 Oct 2019 08:55:12	S	Std
0.2 - 1	50.2	1406	-	0.20007471B	PPB	10 Oct 2019 08:57:30	S	Std
2.5 - 1	52.5	14944	-	2.50007471B	PPB	10 Oct 2019 08:59:48	S	Std
5.0 - 1	55.0	31525	-	5.00007471B	PPB	10 Oct 2019 09:02:05	S	Std
7.5 - 1	57.5	46578	-	7.50007471B	PPB	10 Oct 2019 09:04:23	S	Std
10.0 - 1	510.0	62379	-	10.00007471B	PPB	10 Oct 2019 09:06:40	S	Std
ICV48 - 1	ICV48	23599	3.7906	-7471B	PPB	10 Oct 2019 09:09:32	U	SMPL
ICB48 - 1	ICB48	47	0.0136	-7471B	PPB	10 Oct 2019 09:11:48	U	SMPL
CCV93 - 1	CCV93	31384	5.0390	-7471B	PPB	10 Oct 2019 09:14:04	U	SMPL
CCB93 - 1	CCB93	19	0.0091	-7471B	PPB	10 Oct 2019 09:16:20	U	SMPL
CRA - 1	CRA	1386	0.2284	-7471B	PPB	10 Oct 2019 09:18:36	U	SMPL
HighStd - 1	HighStd	62233	9.9862	-7471B	PPB	10 Oct 2019 09:20:51	U	SMPL
ChkStd - 1	ChkStd	41362	6.6392	-7471B	PPB	10 Oct 2019 09:23:07	U	SMPL
PB123821BL - 1	PBS	51	0.0143	-7471B	PPB	10 Oct 2019 09:25:24	U	SMPL
PB123821BS - 1	LCSS	22363	3.5924	-7471B	PPB	10 Oct 2019 09:30:18	U	SMPL
K5147-01 - 1	OK-03-100719	1716	0.2813	-7471B	PPB	10 Oct 2019 09:32:34	U	SMPL
K5152-01 - 1	SU-02-100719	1593	0.2615	-7471B	PPB	10 Oct 2019 09:34:51	U	SMPL
K5238-01 - 1	TP-COMP	2899	0.4710	-7471B	PPB	10 Oct 2019 09:37:08	U	SMPL
K5239-01 - 1	STONE-COMP	289	0.0524	-7471B	PPB	10 Oct 2019 09:39:26	U	SMPL
K5281-01 - 1	FK-PS-01-062	3546	0.5747	-7471B	PPB	10 Oct 2019 09:41:42	U	SMPL
CCV94 - 1	CCV94	31296	5.0249	-7471B	PPB	10 Oct 2019 09:43:58	U	SMPL
CCB94 - 1	CCB94	34	0.0115	-7471B	PPB	10 Oct 2019 09:46:15	U	SMPL
K5284-01 - 1	FK-EF-01-016-ABCD	10828	1.7425	-7471B	PPB	10 Oct 2019 09:48:31	U	SMPL
K5285-03 - 1	TP-1-S	1083	0.1798	-7471B	PPB	10 Oct 2019 09:50:47	U	SMPL
K5285-03DUP - 1	TP-1-SDUP	1124	0.1863	-7471B	PPB	10 Oct 2019 09:53:03	U	SMPL
K5285-03MS - 1	TP-1-SMS	23262	3.7365	-7471B	PPB	10 Oct 2019 09:55:19	U	SMPL
K5285-03MSD - 1	TP-1-SMSD	23267	3.7373	-7471B	PPB	10 Oct 2019 09:57:36	U	SMPL
K5285-07 - 1	TP-1-D	611	0.1041	-7471B	PPB	10 Oct 2019 09:59:53	U	SMPL
K5285-11 - 1	TP-2-S	23965	3.8493	-7471B	PPB	10 Oct 2019 10:02:10	U	SMPL
K5285-15 - 1	TP-2-D	508	0.0875	-7471B	PPB	10 Oct 2019 10:04:27	U	SMPL
K5286-01 - 1	E.OUTFALL-CREEK-SOIL-SP	62096	9.9642	-7471B	PPB	10 Oct 2019 10:06:44	U	SMPL
PB123822BL - 1	PBS	25	0.0101	-7471B	PPB	10 Oct 2019 10:09:01	U	SMPL
CCV95 - 1	CCV95	31183	5.0068	-7471B	PPB	10 Oct 2019 10:11:18	U	SMPL
CCB95 - 1	CCB95	86	0.0199	-7471B	PPB	10 Oct 2019 10:16:53	U	SMPL
PB123822BS - 1	LCSS	22007	3.5353	-7471B	PPB	10 Oct 2019 10:19:09	U	SMPL
K5145-01 - 1	HD-01-100919	1285	0.2122	-7471B	PPB	10 Oct 2019 10:21:25	U	SMPL
K5145-01DUP - 1	HD-01-100919DUP	1324	0.2184	-7471B	PPB	10 Oct 2019 10:23:40	U	SMPL
K5145-01MS - 1	HD-01-100919MS	22959	3.6879	-7471B	PPB	10 Oct 2019 10:25:56	U	SMPL
K5145-01MSD - 1	HD-01-100919MSD	23755	3.8156	-7471B	PPB	10 Oct 2019 10:28:13	U	SMPL
K5292-01 - 1	20190850-COMPOSITE-B	15922	2.5594	-7471B	PPB	10 Oct 2019 10:30:30	U	SMPL
K5292-02 - 1	20190853-COMPOSITE-E	35098	5.6346	-7471B	PPB	10 Oct 2019 10:32:48	U	SMPL
K5292-03 - 1	20190855-AMEND-COMP-B	12777	2.0551	-7471B	PPB	10 Oct 2019 10:35:05	U	SMPL
K5292-04 - 1	20190857-AMEND-COMP-D	4902	0.7922	-7471B	PPB	10 Oct 2019 10:37:23	U	SMPL
K5292-05 - 1	20190858-AMEND-COMP-E	11962	1.9244	-7471B	PPB	10 Oct 2019 10:39:39	U	SMPL
CCV96 - 1	CCV96	30899	4.9613	-7471B	PPB	10 Oct 2019 10:41:56	U	SMPL
CCB96 - 1	CCB96	35	0.0117	-7471B	PPB	10 Oct 2019 10:44:13	U	SMPL
K5293-01 - 1	KEARNY-TOPSOIL	3073	0.4989	-7471B	PPB	10 Oct 2019 10:46:30	U	SMPL
K5297-04 - 1	TP-1	4334	0.7011	-7471B	PPB	10 Oct 2019 10:48:47	U	SMPL
K5297-06 - 1	TP-2	12292	1.9773	-7471B	PPB	10 Oct 2019 10:51:03	U	SMPL
K5297-08 - 1	TP-3	5903	0.9527	-7471B	PPB	10 Oct 2019 10:53:19	U	SMPL
K5297-10 - 1	TP-4	3203	0.5197	-7471B	PPB	10 Oct 2019 10:55:35	U	SMPL
K5297-12 - 1	TP-5	4609	0.7452	-7471B	PPB	10 Oct 2019 10:57:52	U	SMPL
K5297-14 - 1	TP-6	10502	1.6903	-7471B	PPB	10 Oct 2019 11:00:09	U	SMPL
K5297-16 - 1	TP-7	3758	0.6087	-7471B	PPB	10 Oct 2019 11:02:27	U	SMPL
K5298-01 - 1	TP-7	619	0.1053	-7471B	PPB	10 Oct 2019 11:04:44	U	SMPL
K5298-02 - 1	TP-8	403	0.0707	-7471B	PPB	10 Oct 2019 11:07:01	U	SMPL
CCV97 - 1	CCV97	31062	4.9874	-7471B	PPB	10 Oct 2019 11:09:18	U	SMPL
CCB97 - 1	CCB97	36	0.0119	-7471B	PPB	10 Oct 2019 11:11:34	U	SMPL
K5298-03 - 1	TP-9	374	0.0661	-7471B	PPB	10 Oct 2019 11:13:51	U	SMPL
K5298-04 - 1	TP10	747	0.1259	-7471B	PPB	10 Oct 2019 11:16:07	U	SMPL
K5298-05 - 1	TP-11	4604	0.7444	-7471B	PPB	10 Oct 2019 11:18:23	U	SMPL
K5300-03 - 1	TP-18A-S	958	0.1597	-7471B	PPB	10 Oct 2019 11:20:39	U	SMPL
K5300-07 - 1	TP-18A-D	592	0.1010	-7471B	PPB	10 Oct 2019 11:22:56	U	SMPL
K5285-03LX5 - 1		221	0.0415	-7471B	PPB	10 Oct 2019 11:25:13	U	SMPL
K5285-03A - 1		22851	3.6706	-7471B	PPB	10 Oct 2019 11:27:30	U	SMPL
K5145-01LX5 - 1		257	0.0473	-7471B	PPB	10 Oct 2019 11:29:47	U	SMPL
K5145-01A - 1		23539	3.7810	-7471B	PPB	10 Oct 2019 11:32:05	U	SMPL
CCV98 - 1	CCV98	31159	5.0030	-7471B	PPB	10 Oct 2019 11:34:22	U	SMPL
CCB98 - 1	CCB98	18	0.0090	-7471B	PPB	10 Oct 2019 11:36:38	U	SMPL