


LBI05645

7470A

INSTRUMENT ID : CUI

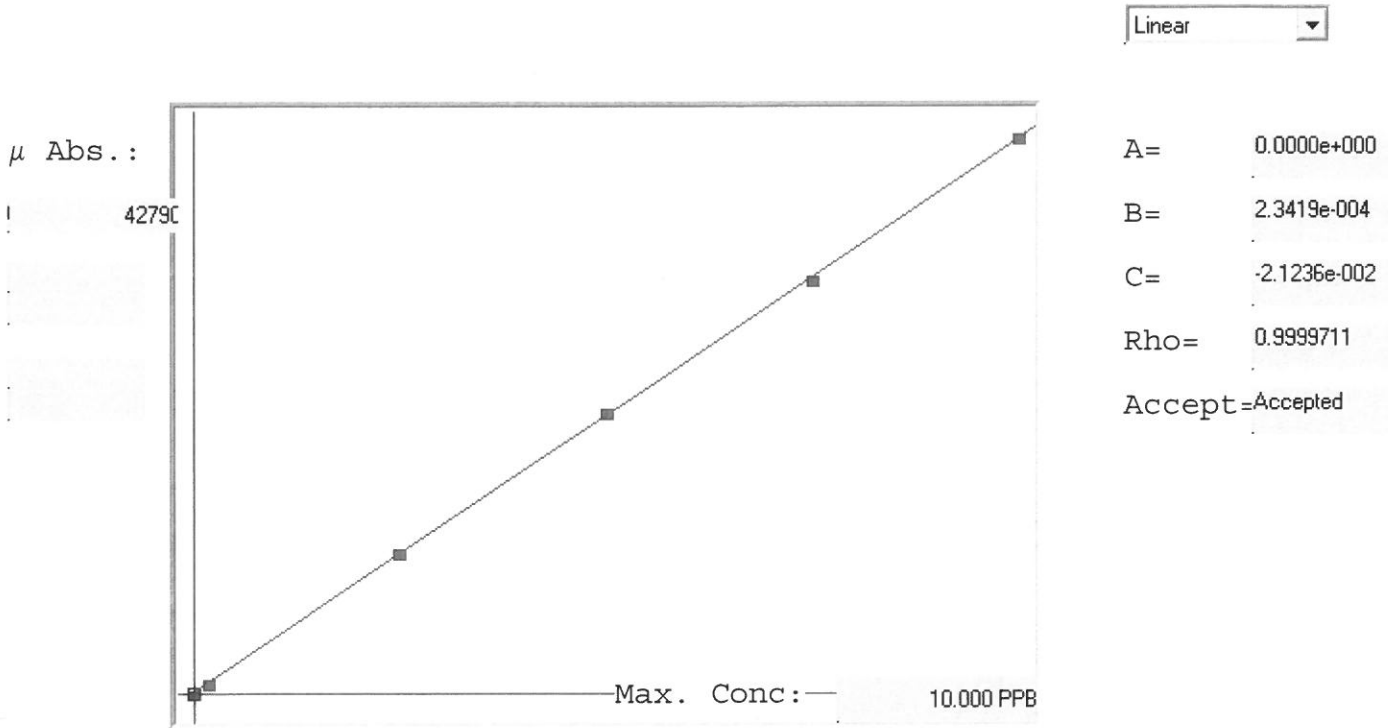

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.003	-0.003	77	0.000	77				
0.2	0.200	0.178	-0.022	851	0.0 %	851				
2.5	2.500	2.512	0.012	10817	0.0 %	10817				
5.0	5.000	5.051	0.051	21660	0.0 %	21660				
7.5	7.500	7.462	-0.038	31953	0.0 %	31953				
10.0	10.000	10.000	-0.000	42790	0.0 %	42790				

LB105645 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 11 Oct 2019 14:52:25			
Sample ID	Extended ID	µ Abs.	Conc.	Std ConcMethod	Units	Date	Type
0.0 - 1	50-0	77	-	0.00007470A	PPB	11 Oct 2019 15:00:28	S Std
0.2 - 1	50-2	851	-	0.20007470A	PPB	11 Oct 2019 15:02:37	S Std
2.5 - 1	52-5	10817	-	2.50007470A	PPB	11 Oct 2019 15:04:46	S Std
5.0 - 1	55-0	21660	-	5.00007470A	PPB	11 Oct 2019 15:06:54	S Std
7.5 - 1	57-5	31953	-	7.50007470A	PPB	11 Oct 2019 15:09:03	S Std
10.0 - 1	50-0	42790	-	10.00007470A	PPB	11 Oct 2019 15:11:11	S Std
ICV52 - 1	ICV52	15801	3.6792	-7470A	PPB	11 Oct 2019 15:17:01	U SMPL
ICB52 - 1	ICB52	16	-0.0175	-7470A	PPB	11 Oct 2019 15:19:08	U SMPL
CCV15 - 1	CCV15	21415	4.9940	-7470A	PPB	11 Oct 2019 15:21:14	U SMPL
CCB15 - 1	CCB15	19	-0.0168	-7470A	PPB	11 Oct 2019 15:23:21	U SMPL
CRA - 1	CRA	844	0.1764	-7470A	PPB	11 Oct 2019 15:25:28	U SMPL
HighStd - 1	HighStd	43065	10.0643	-7470A	PPB	11 Oct 2019 15:27:35	U SMPL
ChkStd - 1	ChkStd	30269	7.0675	-7470A	PPB	11 Oct 2019 15:29:42	U SMPL
PB123902BL - 1	PBW	8	-0.0194	-7470A	PPB	11 Oct 2019 15:31:50	U SMPL
PB123902BS - 1	LCSW	17240	4.0162	-7470A	PPB	11 Oct 2019 15:33:58	U SMPL
K5145-03 - 1	HD-01-100919	11	-0.0187	-7470A	PPB	11 Oct 2019 15:36:06	U SMPL
K5145-03DUP - 1	HD-01-100919DUP	30	-0.0142	-7470A	PPB	11 Oct 2019 15:38:14	U SMPL
K5145-03MS - 1	HD-01-100919MS	17313	4.0333	-7470A	PPB	11 Oct 2019 15:40:23	U SMPL
K5145-03MSD - 1	HD-01-100919MSD	17340	4.0397	-7470A	PPB	11 Oct 2019 15:42:32	U SMPL
K5297-05 - 1	TP-1	47	-0.0102	-7470A	PPB	11 Oct 2019 15:44:39	U SMPL
CCV16 - 1	CCV16	21387	4.9874	-7470A	PPB	11 Oct 2019 15:46:47	U SMPL
CCB16 - 1	CCB16	30	-0.0142	-7470A	PPB	11 Oct 2019 15:48:54	U SMPL
K5297-07 - 1	TP-2	53	-0.0088	-7470A	PPB	11 Oct 2019 15:51:01	U SMPL
K5297-09 - 1	TP-3	34	-0.0133	-7470A	PPB	11 Oct 2019 15:53:08	U SMPL
K5297-11 - 1	TP-4	39	-0.0121	-7470A	PPB	11 Oct 2019 15:55:15	U SMPL
K5297-13 - 1	TP-5	30	-0.0142	-7470A	PPB	11 Oct 2019 15:57:22	U SMPL
K5297-15 - 1	TP-6	40	-0.0119	-7470A	PPB	11 Oct 2019 15:59:30	U SMPL
K5297-17 - 1	TP-7	51	-0.0093	-7470A	PPB	11 Oct 2019 16:01:38	U SMPL
K5300-04 - 1	TP-18A-S	58	-0.0077	-7470A	PPB	11 Oct 2019 16:03:46	U SMPL
K5300-08 - 1	TP-18A-D	44	-0.0109	-7470A	PPB	11 Oct 2019 16:05:54	U SMPL
PB123903BL - 1	PBW	54	-0.0086	-7470A	PPB	11 Oct 2019 16:08:02	U SMPL
PB123903BS - 1	LCSW	17126	3.9895	-7470A	PPB	11 Oct 2019 16:10:09	U SMPL
CCV17 - 1	CCV17	21186	4.9404	-7470A	PPB	11 Oct 2019 16:12:15	U SMPL
CCB17 - 1	CCB17	17	-0.0173	-7470A	PPB	11 Oct 2019 16:14:01	U SMPL
K4660-04 - 1	TP-1-GROUNDWATER	37	-0.0126	-7470A	PPB	11 Oct 2019 16:16:07	U SMPL
K4660-04DUP - 1	TP-1-GROUNDWATERDUP	43	-0.0112	-7470A	PPB	11 Oct 2019 16:18:15	U SMPL
K4660-04MS - 1	TP-1-GROUNDWATERMS	17765	4.1392	-7470A	PPB	11 Oct 2019 16:20:22	U SMPL
K4660-04MSD - 1	TP-1-GROUNDWATERMSD	18129	4.2244	-7470A	PPB	11 Oct 2019 16:22:29	U SMPL
PB123904BL - 1	PBW	8	-0.0194	-7470A	PPB	11 Oct 2019 16:24:36	U SMPL
PB123904BS - 1	LCSW	17216	4.0106	-7470A	PPB	11 Oct 2019 16:26:43	U SMPL
K5149-06 - 1	EO-02-101019	30	-0.0142	-7470A	PPB	11 Oct 2019 16:28:50	U SMPL
K5149-06DUP - 1	EO-02-101019DUP	45	-0.0107	-7470A	PPB	11 Oct 2019 16:31:03	U SMPL
K5149-06MS - 1	EO-02-101019MS	16158	3.7628	-7470A	PPB	11 Oct 2019 16:33:12	U SMPL
K5149-06MSD - 1	EO-02-101019MSD	16272	3.7895	-7470A	PPB	11 Oct 2019 16:35:19	U SMPL
CCV18 - 1	CCV18	20896	4.8724	-7470A	PPB	11 Oct 2019 16:37:27	U SMPL
CCB18 - 1	CCB18	-4	-0.0222	-7470A	PPB	11 Oct 2019 16:39:34	U SMPL
K5176-24 - 1	40166	38	-0.0123	-7470A	PPB	11 Oct 2019 16:41:41	U SMPL
K5266-04 - 1	RAW-DISCRETE-CORE-C-1	36	-0.0128	-7470A	PPB	11 Oct 2019 16:43:48	U SMPL
K5266-05 - 1	RAW-DISCRETE-CORE-C-3	49	-0.0098	-7470A	PPB	11 Oct 2019 16:45:55	U SMPL
K5316-02 - 1	TP-8	52	-0.0091	-7470A	PPB	11 Oct 2019 16:48:02	U SMPL
K5316-04 - 1	TP-9	52	-0.0091	-7470A	PPB	11 Oct 2019 16:50:09	U SMPL
K5316-06 - 1	TP-10	37	-0.0126	-7470A	PPB	11 Oct 2019 16:52:16	U SMPL
K5316-08 - 1	TP-11	36	-0.0128	-7470A	PPB	11 Oct 2019 16:54:23	U SMPL
K5323-02 - 1	TP-1	53	-0.0088	-7470A	PPB	11 Oct 2019 16:56:30	U SMPL
K5323-04 - 1	TP-2	38	-0.0123	-7470A	PPB	11 Oct 2019 16:58:37	U SMPL
K5323-06 - 1	TP-3	108	0.0041	-7470A	PPB	11 Oct 2019 17:00:44	U SMPL
CCV19 - 1	CCV19	21436	4.9989	-7470A	PPB	11 Oct 2019 17:02:51	U SMPL
CCB19 - 1	CCB19	30	-0.0142	-7470A	PPB	11 Oct 2019 17:04:58	U SMPL
K5323-08 - 1	TP-4	64	-0.0062	-7470A	PPB	11 Oct 2019 17:07:05	U SMPL
PB123905BL - 1	PBW	24	-0.0156	-7470A	PPB	11 Oct 2019 17:09:12	U SMPL
PB123905BS - 1	LCSW	16041	3.7354	-7470A	PPB	11 Oct 2019 17:11:19	U SMPL
K5266-08 - 1	20190883-FIELD-BLANK	11	-0.0187	-7470A	PPB	11 Oct 2019 17:13:26	U SMPL
K5297-03 - 1	HH-WATER	457	0.0858	-7470A	PPB	11 Oct 2019 17:15:33	U SMPL
K5297-03DUP - 1	HH-WATERDUP	559	0.1097	-7470A	PPB	11 Oct 2019 17:17:40	U SMPL
K5297-03MS - 1	HH-WATERMS	19113	4.4549	-7470A	PPB	11 Oct 2019 17:19:47	U SMPL
K5297-03MSD - 1	HH-WATERMSD	19024	4.4340	-7470A	PPB	11 Oct 2019 17:21:54	U SMPL
PB123902TB - 1	PB123805TB	28	-0.0147	-7470A	PPB	11 Oct 2019 17:24:01	U SMPL
PB123903TB - 1	PB123806TB	52	-0.0091	-7470A	PPB	11 Oct 2019 17:26:08	U SMPL
CCV20 - 1	CCV20	21812	5.0870	-7470A	PPB	11 Oct 2019 17:28:15	U SMPL
CCB20 - 1	CCB20	0	-0.0212	-7470A	PPB	11 Oct 2019 17:30:22	U SMPL
PB123904TB - 1	PB123846TB	22	-0.0161	-7470A	PPB	11 Oct 2019 17:32:29	U SMPL
K5145-03LX5 - 1		-5	-0.0224	-7470A	PPB	11 Oct 2019 17:34:36	U SMPL
K5145-03A - 1		17089	3.9809	-7470A	PPB	11 Oct 2019 17:36:43	U SMPL
K4660-04LX5 - 1		-11	-0.0238	-7470A	PPB	11 Oct 2019 17:38:50	U SMPL
K4660-04A - 1		17943	4.1809	-7470A	PPB	11 Oct 2019 17:40:57	U SMPL
K5149-06LX5 - 1		-4	-0.0222	-7470A	PPB	11 Oct 2019 17:43:04	U SMPL
K5149-06A - 1		16465	3.8347	-7470A	PPB	11 Oct 2019 17:45:11	U SMPL
K5297-03LX5 - 1		77	-0.0032	-7470A	PPB	11 Oct 2019 17:47:18	U SMPL
K5297-03A - 1		19020	4.4331	-7470A	PPB	11 Oct 2019 17:49:25	U SMPL
CCV21 - 1	CCV21	21529	5.0207	-7470A	PPB	11 Oct 2019 17:51:32	U SMPL
CCB21 - 1	CCB21	13	-0.0182	-7470A	PPB	11 Oct 2019 17:53:39	U SMPL