


LB105670

7471B

INSTRUMENT ID : CV1

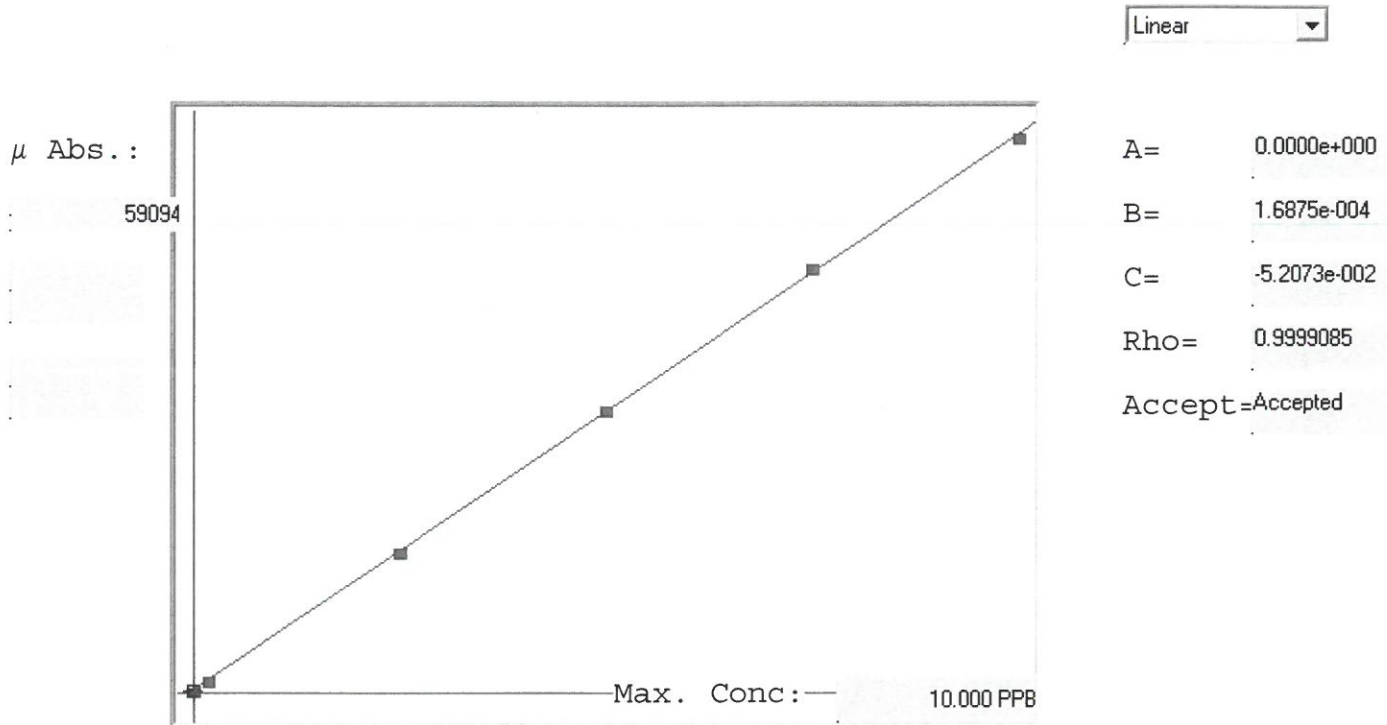

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.017	-0.017	210	0.000	210				
0.2	0.200	0.180	-0.020	1375	0.0 %	1375				
2.5	2.500	2.496	-0.004	15097	0.0 %	15097				
5.0	5.000	5.043	0.043	30195	0.0 %	30195				
7.5	7.500	7.577	0.077	45211	0.0 %	45211				
10.0	10.000	9.920	-0.080	59094	0.0 %	59094				

LB105670 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 14 Oct 2019 09:30:40				
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	50.0	210	-	0.00007471B	PPB		14 Oct 2019 09:54:48	S Std
0.2 - 1	50.2	1375	-	0.20007471B	PPB		14 Oct 2019 09:57:13	S Std
2.5 - 1	52.5	15097	-	2.50007471B	PPB		14 Oct 2019 09:59:31	S Std
5.0 - 1	55.0	30195	-	5.00007471B	PPB		14 Oct 2019 10:01:49	S Std
7.5 - 1	57.5	45211	-	7.50007471B	PPB		14 Oct 2019 10:04:06	S Std
10.0 - 1	510.0	59094	-	10.00007471B	PPB		14 Oct 2019 10:06:24	S Std
ICV53 - 1	ICV53	22061	3.6708	-7471B	PPB		14 Oct 2019 10:09:08	U SMPL
ICB53 - 1	ICB53	194	-0.0193	-7471B	PPB		14 Oct 2019 10:11:24	U SMPL
CCV22 - 1	CCV22	30427	5.0826	-7471B	PPB		14 Oct 2019 10:13:40	U SMPL
CCB22 - 1	CCB22	164	-0.0244	-7471B	PPB		14 Oct 2019 10:15:57	U SMPL
CRA - 1	CRA	1403	0.1847	-7471B	PPB		14 Oct 2019 10:18:14	U SMPL
HighStd - 1	HighStd	59277	9.9511	-7471B	PPB		14 Oct 2019 10:20:30	U SMPL
ChkStd - 1	ChkStd	42417	7.1059	-7471B	PPB		14 Oct 2019 10:22:46	U SMPL
PB123938BL - 1	PBS	233	-0.0128	-7471B	PPB		14 Oct 2019 10:25:04	U SMPL
PB123938BS - 1	LCSS	22255	3.7035	-7471B	PPB		14 Oct 2019 10:27:21	U SMPL
K5149-01 - 1	EO-02-101019	19502	3.2390	-7471B	PPB		14 Oct 2019 10:29:38	U SMPL
K5149-01DUP - 1	EO-02-101019DUP	19546	3.2464	-7471B	PPB		14 Oct 2019 10:31:55	U SMPL
K5149-01MSD - 1	EO-02-101019MSD	45710	7.6616	-7471B	PPB		14 Oct 2019 10:36:32	U SMPL
K5266-01 - 1	20190849-COMPOSITE-A	28215	4.7093	-7471B	PPB		14 Oct 2019 10:38:49	U SMPL
CCV23 - 1	CCV23	30445	5.0856	-7471B	PPB		14 Oct 2019 10:41:06	U SMPL
CCB23 - 1	CCB23	182	-0.0214	-7471B	PPB		14 Oct 2019 10:43:23	U SMPL
K5266-02 - 1	20190851-COMPOSITE-C	17856	2.9612	-7471B	PPB		14 Oct 2019 10:45:39	U SMPL
K5266-03 - 1	20190845-D-2	26550	4.4283	-7471B	PPB		14 Oct 2019 10:47:56	U SMPL
K5266-06 - 1	20190854-AMENDED-COMP-A	23021	3.8328	-7471B	PPB		14 Oct 2019 10:50:12	U SMPL
K5266-07 - 1	20190856-AMENDED-COMP-C	31638	5.2869	-7471B	PPB		14 Oct 2019 10:52:29	U SMPL
K5316-01 - 1	TP-8	21529	3.5810	-7471B	PPB		14 Oct 2019 10:54:46	U SMPL
K5316-03 - 1	TP-9	10498	1.7195	-7471B	PPB		14 Oct 2019 10:57:03	U SMPL
K5316-05 - 1	TP-10	9099	1.4834	-7471B	PPB		14 Oct 2019 10:59:23	U SMPL
K5316-07 - 1	TP-11	10139	1.6589	-7471B	PPB		14 Oct 2019 11:01:41	U SMPL
K5323-01 - 1	TP-1	4718	0.7441	-7471B	PPB		14 Oct 2019 11:03:59	U SMPL
K5324-01 - 1	SOIL-PILE	1571	0.2130	-7471B	PPB		14 Oct 2019 11:06:15	U SMPL
CCV24 - 1	CCV24	30951	5.1710	-7471B	PPB		14 Oct 2019 11:08:32	U SMPL
CCB24 - 1	CCB24	216	-0.0156	-7471B	PPB		14 Oct 2019 11:10:48	U SMPL
K5325-01 - 1	10-10-A	1137	0.1398	-7471B	PPB		14 Oct 2019 11:13:04	U SMPL
K5325-02 - 1	10-10-B	1099	0.1334	-7471B	PPB		14 Oct 2019 11:15:20	U SMPL
K5325-03 - 1	10-10-C	983	0.1138	-7471B	PPB		14 Oct 2019 11:17:36	U SMPL
K5325-04 - 1	10-10-D	605	0.0500	-7471B	PPB		14 Oct 2019 11:19:52	U SMPL
K5325-05 - 1	10-10-E	745	0.0736	-7471B	PPB		14 Oct 2019 11:26:51	U SMPL
K5325-07 - 1	10-10-F	569	0.0439	-7471B	PPB		14 Oct 2019 11:29:07	U SMPL
K5325-08 - 1	10-10-G	2028	0.2902	-7471B	PPB		14 Oct 2019 11:31:25	U SMPL
K5325-09 - 1	10-10-H	1322	0.1710	-7471B	PPB		14 Oct 2019 11:33:42	U SMPL
K5325-10 - 1	10-10-I	691	0.0645	-7471B	PPB		14 Oct 2019 11:36:01	U SMPL
K5325-11 - 1	10-10-J	1364	0.1781	-7471B	PPB		14 Oct 2019 11:38:18	U SMPL
CCV25 - 1	CCV25	31325	5.2341	-7471B	PPB		14 Oct 2019 11:40:34	U SMPL
CCB25 - 1	CCB25	173	-0.0229	-7471B	PPB		14 Oct 2019 11:42:50	U SMPL
PB123939BL - 1	PBS	-20	-0.0554	-7471B	PPB		14 Oct 2019 11:45:07	U SMPL
PB123939BS - 1	LCSS	22447	3.7359	-7471B	PPB		14 Oct 2019 11:47:22	U SMPL
K5148-05 - 1	OR-03-101119	5160	0.8187	-7471B	PPB		14 Oct 2019 11:49:37	U SMPL
K5148-05DUP - 1	OR-03-101119DUP	4090	0.6381	-7471B	PPB		14 Oct 2019 11:51:54	U SMPL
K5148-05MS - 1	OR-03-101119MS	25190	4.1988	-7471B	PPB		14 Oct 2019 11:54:12	U SMPL
K5148-05MSD - 1	OR-03-101119MSD	24886	4.1475	-7471B	PPB		14 Oct 2019 11:56:32	U SMPL
K5160-03 - 1	CSA-3-2	1477	0.1972	-7471B	PPB		14 Oct 2019 11:58:49	U SMPL
K5160-05 - 1	CSA-3-1	1865	0.2627	-7471B	PPB		14 Oct 2019 12:01:07	U SMPL
K5323-03 - 1	TP-2	4315	0.6761	-7471B	PPB		14 Oct 2019 12:03:25	U SMPL
K5323-05 - 1	TP-3	3227	0.4925	-7471B	PPB		14 Oct 2019 12:05:42	U SMPL
CCV26 - 1	CCV26	31572	5.2758	-7471B	PPB		14 Oct 2019 12:07:58	U SMPL
CCB26 - 1	CCB26	341	0.0055	-7471B	PPB		14 Oct 2019 12:10:15	U SMPL
K5323-07 - 1	TP-4	3618	0.5585	-7471B	PPB		14 Oct 2019 12:14:06	U SMPL
K5350-01 - 1	VNJ-209	4370	0.6854	-7471B	PPB		14 Oct 2019 12:16:23	U SMPL
K5350-03 - 1	VNJ-11935	506	0.0333	-7471B	PPB		14 Oct 2019 12:18:39	U SMPL
K5350-05 - 1	VNJ-230	762	0.0765	-7471B	PPB		14 Oct 2019 12:20:56	U SMPL
K5351-03 - 1	A-FRAME-SOIL	1765	0.2458	-7471B	PPB		14 Oct 2019 12:23:13	U SMPL
K5352-03 - 1	TP-19-S	1541	0.2080	-7471B	PPB		14 Oct 2019 12:25:29	U SMPL
K5352-07 - 1	TP-20A-S	1164	0.1444	-7471B	PPB		14 Oct 2019 12:27:47	U SMPL
K5352-11 - 1	TP-20A-D	1421	0.1877	-7471B	PPB		14 Oct 2019 12:30:04	U SMPL
K5149-01LX5 - 1		4039	0.6295	-7471B	PPB		14 Oct 2019 12:32:22	U SMPL
K5149-01A - 1		46637	7.8181	-7471B	PPB		14 Oct 2019 12:34:38	U SMPL
CCV27 - 1	CCV27	31818	5.3173	-7471B	PPB		14 Oct 2019 12:36:55	U SMPL
CCB27 - 1	CCB27	200	-0.0183	-7471B	PPB		14 Oct 2019 12:39:12	U SMPL
K5148-05LX5 - 1		1161	0.1438	-7471B	PPB		14 Oct 2019 12:41:29	U SMPL
K5148-05A - 1		24986	4.1644	-7471B	PPB		14 Oct 2019 12:43:46	U SMPL
K5149-01MS - 1	EO-02-101019MS	46368	7.7727	-7471B	PPB		14 Oct 2019 12:46:03	U SMPL
CCV28 - 1	CCV28	30390	5.0763	-7471B	PPB		14 Oct 2019 12:48:19	U SMPL
CCB28 - 1	CCB28	208	-0.0170	-7471B	PPB		14 Oct 2019 12:50:37	U SMPL