

LB105676

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : CT

Instrument ID : Konelab

10/14/2019 11:57


Test ~~Total~~ CN

Accepted 10/14/2019 8:34

Factor 1129
Bias 0.002

Coeff. of det. 0.999980

Errors

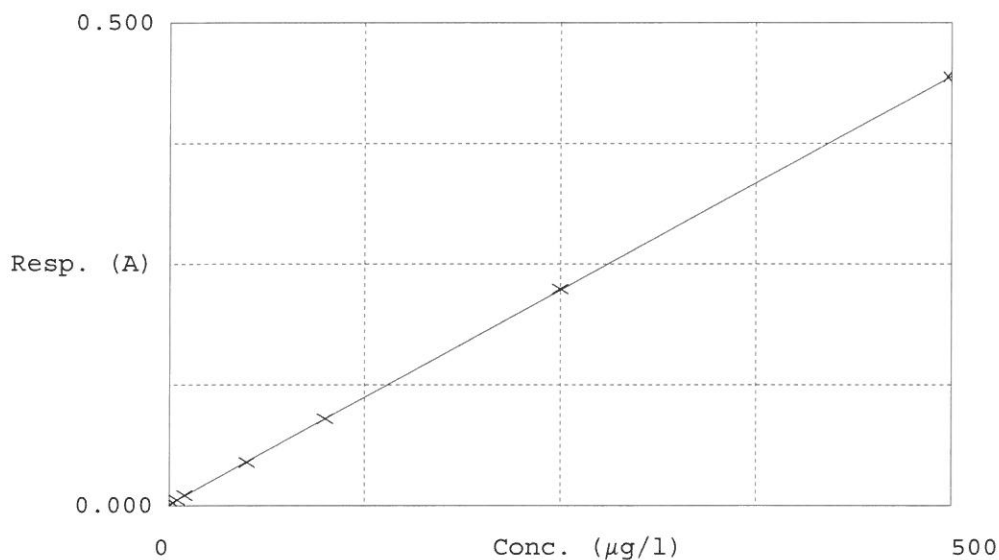

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.3686	0.0000	
2	5.0PPBCN	0.006	5.1598	5.0000	
3	10PPBCN	0.011	10.5798	10.0000	
4	50PPBCN	0.045	48.8474	50.0000	
5	100PPBCN	0.090	99.9683	100.0000	
6	250PPBCN	0.224	251.4098	250.0000	
7	500PPBCN	0.444	499.4035	500.0000	

10/14/19
CT

LB105676

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

10/14/2019 11:52

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	99.059	0.0	0.089	
ICB1	0.399	0.0	0.002	

N	2
Mean	49.729
SD	69.7630
CV%	140.29

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

10/14/2019 11:51

Test: ~~Total~~ ^{SPLP} CN

Sample Id	Result	Dil. 1 +	Response	Errors
-----------	--------	----------	----------	--------

CCV1	CCV4	250.836	0.0	0.224
CCB1	CCB4	0.311	0.0	0.002
	PB123893BL	0.222	0.0	0.002
	PB123893BS	95.293	0.0	0.086
	K5266-13	0.413	0.0	0.002
	K5266-13DUP	0.304	0.0	0.002
	K5266-13MS	3.250	0.0	0.004
	K5266-13MSD	3.414	0.0	0.005
	K5266-14	0.301	0.0	0.002
	CCV5	244.480	0.0	0.218
	CCB5	0.105	0.0	0.002
	K5292-06	2.224	0.0	0.004
	K5292-07	0.604	0.0	0.002
	K5292-08	0.783	0.0	0.002
	CCV6	254.529	0.0	0.227
	CCB6	0.184	0.0	0.002

N	16
Mean	53.578
SD	100.2177
CV%	187.05

CT
10/14/19

Aquakem v. 7.2AQ1

Results from time period:

Mon Oct 14 11:14:00 2019

Mon Oct 14 11:50:06 2019

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	SPLP CN	P	-0.3686	µg/l	10/14/2019 8:34:13	
5.OPPBCN	A	SPLP CN	P	5.1598	µg/l	10/14/2019 8:34:14	
10PPBCN	A	SPLP CN	P	10.5798	µg/l	10/14/2019 8:34:15	
50PPBCN	A	SPLP CN	P	48.8474	µg/l	10/14/2019 8:34:16	
100PPBCN	A	SPLP CN	P	99.9683	µg/l	10/14/2019 8:34:17	
250PPBCN	A	SPLP CN	P	251.4098	µg/l	10/14/2019 8:34:18	
500PPBCN	A	SPLP CN	P	499.4035	µg/l	10/14/2019 8:34:19	
ICV1	S	SPLP CN	P	99.0586	µg/l	10/14/2019 11:14:01	
ICB1	S	SPLP CN	P	0.3988	µg/l	10/14/2019 11:14:02	
CCV1	S	SPLP CN	P	250.8364	µg/l	10/14/2019 11:36:53	
CCB1	S	SPLP CN	P	0.3114	µg/l	10/14/2019 11:36:54	
PB123893BL	S	SPLP CN	P	0.2215	µg/l	10/14/2019 11:44:20	
PB123893BS	S	SPLP CN	P	95.2931	µg/l	10/14/2019 11:44:21	
K5266-13	S	SPLP CN	P	0.4132	µg/l	10/14/2019 11:44:22	
K5266-13DUP	S	SPLP CN	P	0.3038	µg/l	10/14/2019 11:44:23	
K5266-13MS	S	SPLP CN	P	3.2504	µg/l	10/14/2019 11:44:24	
K5266-13MSD	S	SPLP CN	P	3.414	µg/l	10/14/2019 11:44:25	
K5266-14	S	SPLP CN	P	0.3006	µg/l	10/14/2019 11:44:26	
CCV2	S	SPLP CN	P	244.4799	µg/l	10/14/2019 11:44:27	
CCB2	S	SPLP CN	P	0.1054	µg/l	10/14/2019 11:50:00	
K5292-06	S	SPLP CN	P	2.2241	µg/l	10/14/2019 11:50:01	
K5292-07	S	SPLP CN	P	0.6043	µg/l	10/14/2019 11:50:02	
K5292-08	S	SPLP CN	P	0.7828	µg/l	10/14/2019 11:50:03	
CCV3	S	SPLP CN	P	254.5294	µg/l	10/14/2019 11:50:04	
CCB3	S	SPLP CN	P	0.1838	µg/l	10/14/2019 11:50:05	