


LB105707

INSTRUMENT ID: CV1

7470A

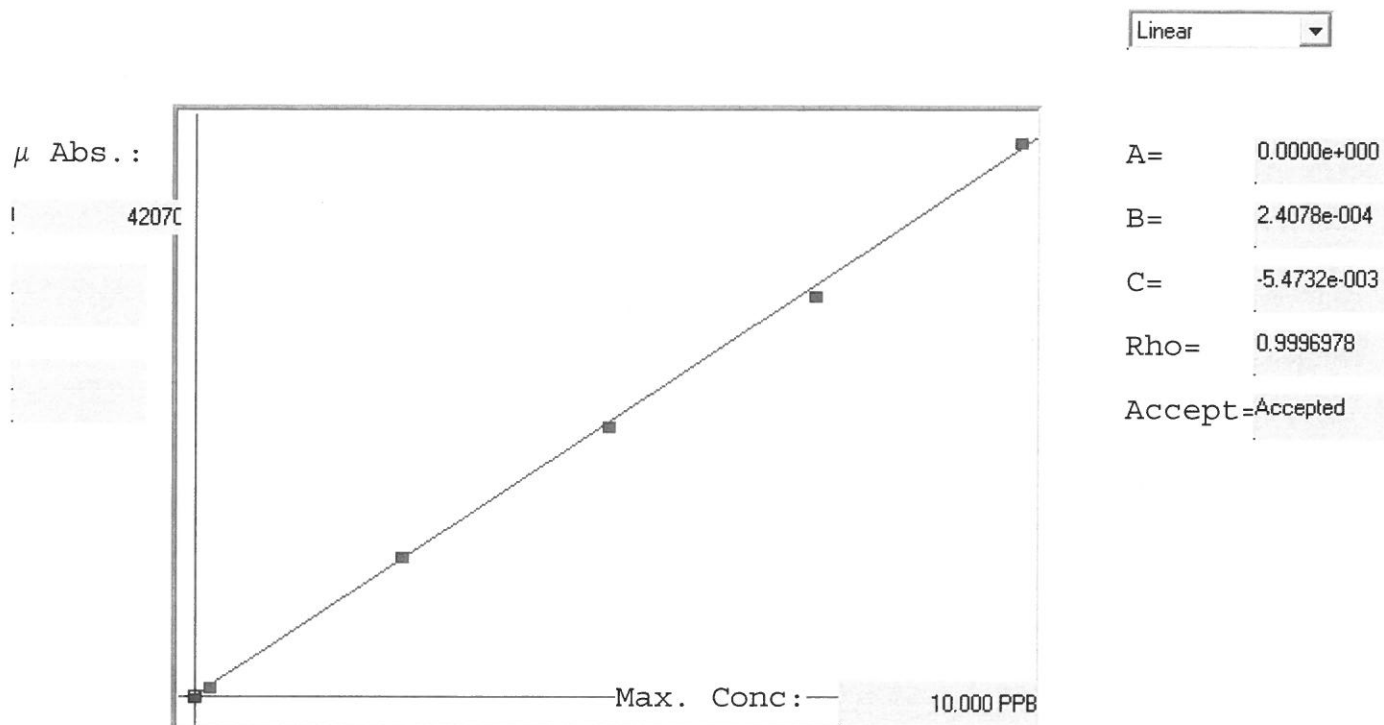

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.017	0.017	95	0.000	95				
0.2	0.200	0.201	0.001	856	0.0 %	856				
2.5	2.500	2.572	0.072	10704	0.0 %	10704				
5.0	5.000	4.946	-0.054	20565	0.0 %	20565				
7.5	7.500	7.340	-0.160	30507	0.0 %	30507				
10.0	10.000	10.124	0.124	42070	0.0 %	42070				

LB105707 INSTRUMENT ID : CV1

Method: 7470A	Operator: Admin	Date of Analysis: 15 Oct 2019 13:54:32							
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	95	-	0.0000	7470A	PPB	15 Oct 2019 13:57:23	S	Std
0.2 - 1	50-2	856	-	0.2000	7470A	PPB	15 Oct 2019 13:59:32	S	Std
2.5 - 1	52-5	10704	-	2.5000	7470A	PPB	15 Oct 2019 14:01:41	S	Std
5.0 - 1	55-0	20565	-	5.0000	7470A	PPB	15 Oct 2019 14:03:49	S	Std
7.5 - 1	57-5	30507	-	7.5000	7470A	PPB	15 Oct 2019 14:05:57	S	Std
10.0 - 1	510-0	42070	-	10.0000	7470A	PPB	15 Oct 2019 14:08:05	S	Std
ICV56 - 1	ICV56	15626	3.7569	-	7470A	PPB	15 Oct 2019 14:14:01	U	SMPL
ICB56 - 1	ICB56	38	0.0037	-	7470A	PPB	15 Oct 2019 14:16:07	U	SMPL
CCV37 - 1	CCV37	20169	4.8508	-	7470A	PPB	15 Oct 2019 14:18:13	U	SMPL
CCB37 - 1	CCB37	29	0.0015	-	7470A	PPB	15 Oct 2019 14:20:20	U	SMPL
CRA - 1	CRA	836	0.1958	-	7470A	PPB	15 Oct 2019 14:22:26	U	SMPL
HighStd - 1	HighStd	42577	10.2461	-	7470A	PPB	15 Oct 2019 14:24:33	U	SMPL
ChkStd - 1	ChkStd	29244	7.0358	-	7470A	PPB	15 Oct 2019 14:26:40	U	SMPL
PB123991BL - 1	PBW	-18	-0.0098	-	7470A	PPB	15 Oct 2019 14:28:47	U	SMPL
PB123991BS - 1	LCSW	17372	4.1773	-	7470A	PPB	15 Oct 2019 14:30:54	U	SMPL
K5148-08 - 1	OR-03-101119	80	0.0138	-	7470A	PPB	15 Oct 2019 14:38:32	U	SMPL
K5148-08DUP - 1	OR-03-101119DUP	52	0.0070	-	7470A	PPB	15 Oct 2019 14:40:40	U	SMPL
K5148-08MS - 1	OR-03-101119MS	17070	4.1046	-	7470A	PPB	15 Oct 2019 14:42:48	U	SMPL
K5148-08MSD - 1	OR-03-101119MSD	16797	4.0389	-	7470A	PPB	15 Oct 2019 14:44:57	U	SMPL
K5176-25 - 1	30464-67	35	0.0030	-	7470A	PPB	15 Oct 2019 14:47:04	U	SMPL
CCV38 - 1	CCV38	20587	4.9514	-	7470A	PPB	15 Oct 2019 14:49:11	U	SMPL
CCB38 - 1	CCB38	1	-0.0052	-	7470A	PPB	15 Oct 2019 14:51:18	U	SMPL
K5335-02 - 1	IDW-GAC2-191010	29	0.0015	-	7470A	PPB	15 Oct 2019 14:53:25	U	SMPL
K5339-01 - 1	SOIL-BIN-1	23	0.0001	-	7470A	PPB	15 Oct 2019 14:55:32	U	SMPL
K5350-02 - 1	VNJ-209	20	-0.0007	-	7470A	PPB	15 Oct 2019 14:57:39	U	SMPL
K5350-04 - 1	VNJ-11935	35	0.0030	-	7470A	PPB	15 Oct 2019 14:59:46	U	SMPL
K5350-06 - 1	VNJ-230	37	0.0034	-	7470A	PPB	15 Oct 2019 15:01:53	U	SMPL
K5352-04 - 1	TP-19-S	59	0.0087	-	7470A	PPB	15 Oct 2019 15:04:01	U	SMPL
K5352-08 - 1	TP-20A-S	48	0.0061	-	7470A	PPB	15 Oct 2019 15:06:08	U	SMPL
K5352-12 - 1	TP-20A-D	36	0.0032	-	7470A	PPB	15 Oct 2019 15:08:16	U	SMPL
PB123994BL - 1	PBW	54	0.0075	-	7470A	PPB	15 Oct 2019 15:10:25	U	SMPL
PB123994BS - 1	LCSW	17120	4.1167	-	7470A	PPB	15 Oct 2019 15:12:31	U	SMPL
CCV39 - 1	CCV39	20497	4.9298	-	7470A	PPB	15 Oct 2019 15:14:38	U	SMPL
CCB39 - 1	CCB39	28	0.0013	-	7470A	PPB	15 Oct 2019 15:16:45	U	SMPL
K5337-01 - 1	HHT-WATER	93	0.0169	-	7470A	PPB	15 Oct 2019 15:18:51	U	SMPL
K5337-01DUP - 1	HHT-WATERDUP	93	0.0169	-	7470A	PPB	15 Oct 2019 15:20:58	U	SMPL
K5337-01MS - 1	HHT-WATERMS	18379	4.4198	-	7470A	PPB	15 Oct 2019 15:23:04	U	SMPL
K5337-01MSD - 1	HHT-WATERMSD	18055	4.3418	-	7470A	PPB	15 Oct 2019 15:25:11	U	SMPL
K5358-03 - 1	20190891-FIELD-BLANK	16	-0.0016	-	7470A	PPB	15 Oct 2019 15:27:18	U	SMPL
PB123991TB - 1	PB123906TB	27	0.0010	-	7470A	PPB	15 Oct 2019 15:29:25	U	SMPL
K5148-08LX5 - 1		15	-0.0019	-	7470A	PPB	15 Oct 2019 15:31:33	U	SMPL
K5148-08A - 1		16748	4.0271	-	7470A	PPB	15 Oct 2019 15:33:41	U	SMPL
K5337-01LX5 - 1		2	-0.0050	-	7470A	PPB	15 Oct 2019 15:35:49	U	SMPL
K5337-01A - 1		18119	4.3572	-	7470A	PPB	15 Oct 2019 15:37:56	U	SMPL
CCV40 - 1	CCV40	21225	5.1050	-	7470A	PPB	15 Oct 2019 15:40:04	U	SMPL
CCB40 - 1	CCB40	38	0.0037	-	7470A	PPB	15 Oct 2019 15:42:11	U	SMPL