

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CS

Instrument ID : Konelab

10/17/2019 14:46


Test Nitrite

Accepted 10/17/2019 11:59

Factor 0.403
Bias 0.008

Coeff. of det. 0.999782

Errors Meas. error

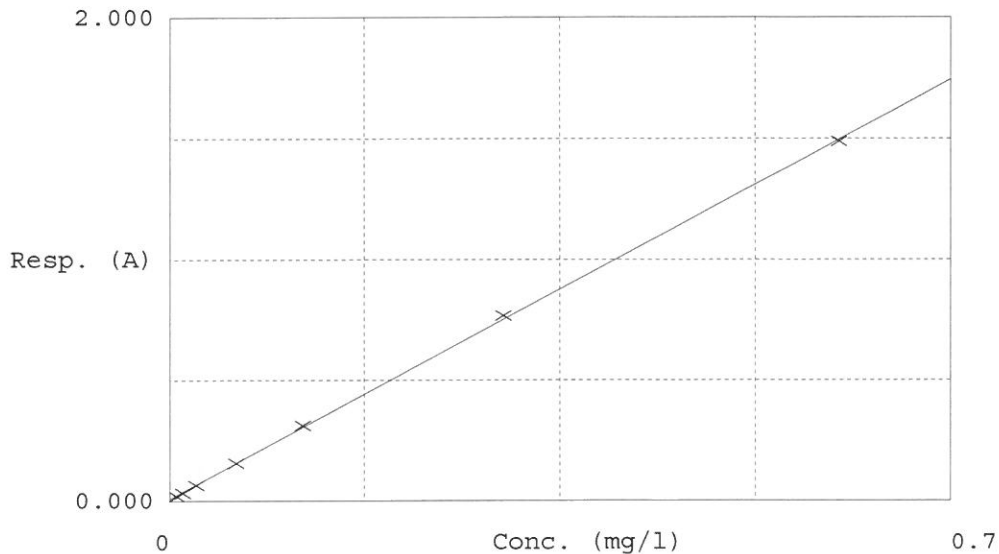

	Calibrator	Response	Calc. con.	Conc.	Errors
1	NITRITE0.6	0.018	0.0039	0.0060	Blank resp. low
2	NITRITE0.6	0.033	0.0100	0.0120	Blank resp. low
3	NITRITE0.6	0.066	0.0232	0.0240	Blank resp. low
4	NITRITE0.6	0.156	0.0597	0.0600	
5	NITRITE0.6	0.313	0.1228	0.1200	Blank resp. low
6	NITRITE0.6	0.767	0.3059	0.3000	
7	NITRITE0.6	1.488	0.5966	0.6000	Blank resp. low

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

10/17/2019 14:39

Test: Nitrite

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.310 ✓	0.0	0.776	Blank resp. low
ICB1	-0.002 ✓	0.0	0.003	Blank resp. low
CCV1	0.301 ✓	0.0	0.755	Blank resp. low
CCB1	-0.002 ✓	0.0	0.003	Blank resp. low
LB105770BL	-0.002	0.0	0.003	Blank resp. low
LB105770BS	0.308	0.0	0.773	Blank resp. low
K5111-07	0.001	0.0	0.011	Blank resp. low
K5111-08	0.004	0.0	0.019	Blank resp. low
CCV2	0.304	0.0	0.762	Blank resp. low
CCB2	-0.002	0.0	0.003	Blank resp. low
N	10			
Mean	0.122			
SD	0.1582			
CV%	129.69			

10/17/19
CT

Aquakem v. 7.2AQ1

Results from time period:

Thu Oct 17 13:46:12 2019

Thu Oct 17 14:17:23 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0061PPM	A	Nitrite	P	0.0039	mg/l	10/17/2019 11:55:42	
0.0122PPM	A	Nitrite	P	0.01	mg/l	10/17/2019 11:55:43	
0.0243PPM	A	Nitrite	P	0.0232	mg/l	10/17/2019 11:55:44	
0.0608PPM	A	Nitrite	P	0.0597	mg/l	10/17/2019 11:55:45	
0.1216PPM	A	Nitrite	P	0.1228	mg/l	10/17/2019 11:55:46	
0.304PPM	A	Nitrite	P	0.3059	mg/l	10/17/2019 11:55:47	
0.608PPM	A	Nitrite	P	0.5966	mg/l	10/17/2019 11:55:48	
ICV1	S	Nitrite	P	0.3095	mg/l	10/17/2019 13:46:12	
ICB1	S	Nitrite	P	-0.0023	mg/l	10/17/2019 13:46:13	
CCV1	S	Nitrite	P	0.3009	mg/l	10/17/2019 13:46:14	
CCB1	S	Nitrite	P	-0.0021	mg/l	10/17/2019 13:46:15	
LB105770BL	S	Nitrite	P	-0.0021	mg/l	10/17/2019 13:46:16	
LB105770BS	S	Nitrite	P	0.3083	mg/l	10/17/2019 13:46:17	
K5111-07	S	Nitrite	P	0.001	mg/l	10/17/2019 13:46:18	
K5111-08	S	Nitrite	P	0.0042	mg/l	10/17/2019 13:46:19	
CCV2	S	Nitrite	P	0.304	mg/l	10/17/2019 13:46:20	
CCB2	S	Nitrite	P	-0.0019	mg/l	10/17/2019 13:46:21	