

=====

Calibration results	Aquakem 7.2AQ1	Page: 1
---------------------	----------------	---------

=====

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : GT

Instrument ID : Konelab

10/17/2019 15:29


Test Phenolics-

Accepted 10/17/2019 15:29

Factor 8.956
Bias 0.011

Coeff. of det. 0.999726

Errors

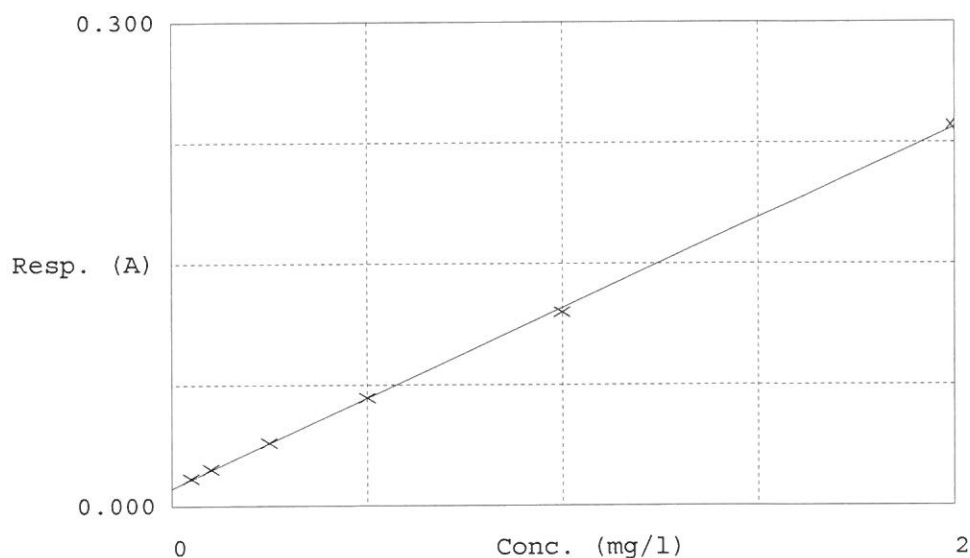

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.017	0.0540	0.0500	
2	Phenol-2	0.023	0.1054	0.1000	
3	Phenol-2	0.039	0.2522	0.2500	
4	Phenol-2	0.067	0.5017	0.5000	
5	Phenol-2	0.120	0.9757	1.0000	
6	Phenol-2	0.236	2.0111	2.0000	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by :



Instrument ID : Konelab

10/17/2019 16:21

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.970 ✓	0.0	0.119	
ICB1	0.006 ✓	0.0	0.012	
CCV1	0.973 ✓	0.0	0.120	
CCB1	0.008 ✓	0.0	0.012	
PB123958BL	0.003	0.0	0.011	
PB123958BS	0.974	0.0	0.120	
K5111-09	0.015 ✓	0.0	0.013	
PB123956BL	0.004	0.0	0.012	
PB123956BS	0.979	0.0	0.120	
K5111-03	0.014 ✓	0.0	0.013	
CCV2	0.977	0.0	0.120	
CCB2	0.002	0.0	0.011	

N	12
Mean	0.410
SD	0.4981
CV%	121.36

Aquakem v. 7.2AQ1

Results from time period:

Thu Oct 17 15:27:55 2019

Thu Oct 17 16:06:41 2019

CT
10/17/19

Sample Id	Sam/Ctr/c	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.054	mg/l	10/17/2019 15:27:55	
0.1PPM	A	Phenolics-	P	0.1054	mg/l	10/17/2019 15:27:56	
0.25PPM	A	Phenolics-	P	0.2522	mg/l	10/17/2019 15:27:57	
0.50PPM	A	Phenolics-	P	0.5017	mg/l	10/17/2019 15:27:58	
1.0PPM	A	Phenolics-	P	0.9757	mg/l	10/17/2019 15:27:59	
2.0PPM	A	Phenolics-	P	2.0111	mg/l	10/17/2019 15:28:00	
ICV1	S	Phenolics-	P	0.9701	mg/l	10/17/2019 16:02:42	
ICB1	S	Phenolics-	P	0.0058	mg/l	10/17/2019 16:02:43	
CCV1	S	Phenolics-	P	0.9734	mg/l	10/17/2019 16:02:44	
CCB1	S	Phenolics-	P	0.0077	mg/l	10/17/2019 16:02:45	
PB123958BL	S	Phenolics-	P	0.0032	mg/l	10/17/2019 16:02:46	
PB123958BS	S	Phenolics-	P	0.9735	mg/l	10/17/2019 16:02:47	
K5111-09	S	Phenolics-	P	0.0145	mg/l	10/17/2019 16:02:48	
PB123956BL	S	Phenolics-	P	0.0041	mg/l	10/17/2019 16:02:50	
PB123956BS	S	Phenolics-	P	0.9792	mg/l	10/17/2019 16:02:51	
K5111-03	S	Phenolics-	P	0.0142	mg/l	10/17/2019 16:02:53	
CCV2	S	Phenolics-	P	0.9767	mg/l	10/17/2019 16:06:40	
CCB2	S	Phenolics-	P	0.0021	mg/l	10/17/2019 16:06:41	