


LB10577S

7471B

INSTRUMENT ID : CV1

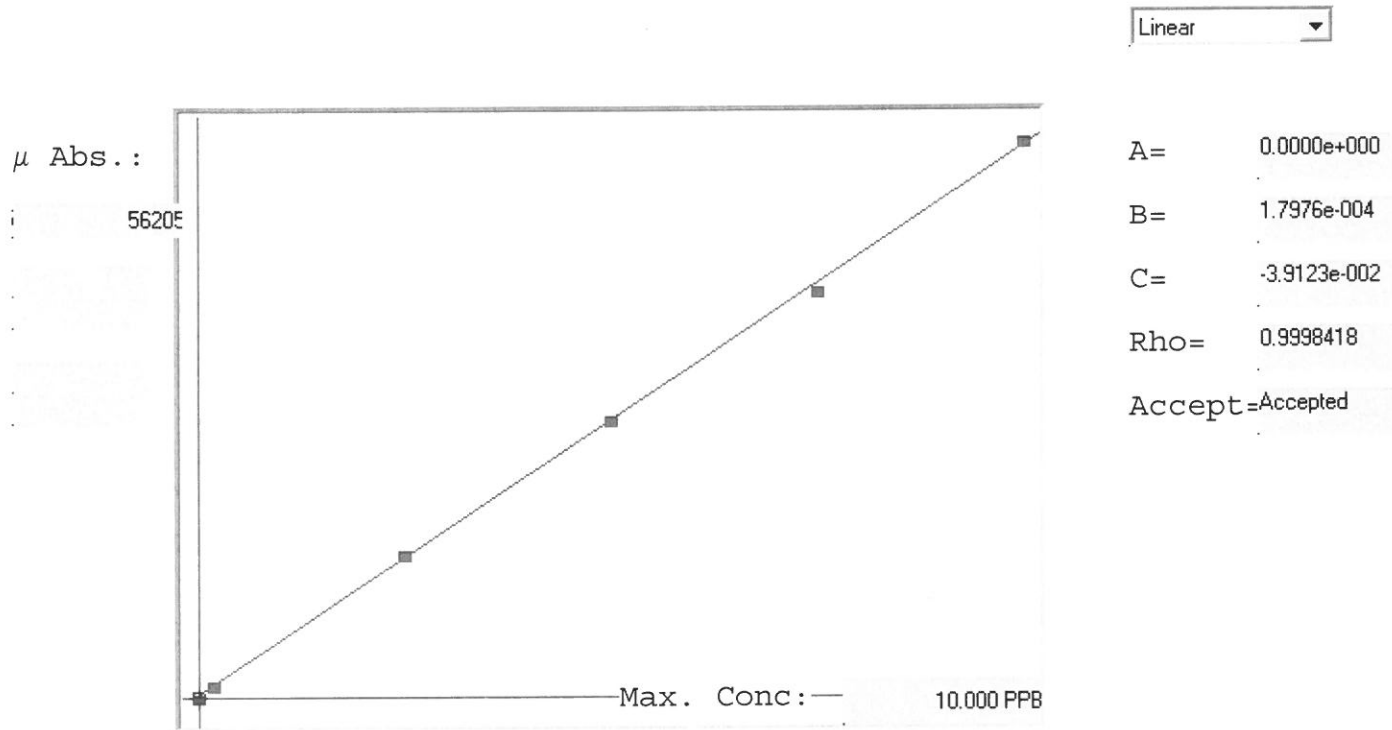

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.018	-0.018	115	0.000	115				
0.2	0.200	0.192	-0.008	1286	0.0 %	1286				
2.5	2.500	2.562	0.062	14468	0.0 %	14468				
5.0	5.000	5.030	0.030	28199	0.0 %	28199				
7.5	7.500	7.371	-0.129	41223	0.0 %	41223				
10.0	10.000	10.064	0.064	56205	0.0 %	56205				

LB105779 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 18 Oct 2019 07:56:34

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	115	-	0.00007471B	PPB		18 Oct 2019 08:23:11	S	Std
0.2 - 1	50-1	1286	-	0.20007471B	PPB		18 Oct 2019 08:25:30	S	Std
2.5 - 1	52-5	14468	-	2.50007471B	PPB		18 Oct 2019 08:27:49	S	Std
5.0 - 1	55-0	28199	-	5.00007471B	PPB		18 Oct 2019 08:30:07	S	Std
7.5 - 1	57-5	41223	-	7.50007471B	PPB		18 Oct 2019 08:33:42	S	Std
10.0 - 1	510-0	56205	-	10.00007471B	PPB		18 Oct 2019 08:39:47	S	Std
ICV61 - 1	ICV61	22122	3.9374	-7471B	PPB		18 Oct 2019 08:42:31	U	SMPL
ICB61 - 1	ICB61	86	-0.0237	-7471B	PPB		18 Oct 2019 08:44:47	U	SMPL
CCV67 - 1	CCV67	28859	5.1485	-7471B	PPB		18 Oct 2019 08:47:02	U	SMPL
CCB67 - 1	CCB67	98	-0.0215	-7471B	PPB		18 Oct 2019 08:49:20	U	SMPL
CRA - 1	CRA	1295	0.1937	-7471B	PPB		18 Oct 2019 08:52:31	U	SMPL
HighStd - 1	HighStd	57199	10.2427	-7471B	PPB		18 Oct 2019 08:54:47	U	SMPL
ChkStd - 1	ChkStd	38603	6.9000	-7471B	PPB		18 Oct 2019 08:57:03	U	SMPL
PB124092BL - 1	PBS	13	-0.0368	-7471B	PPB		18 Oct 2019 08:59:20	U	SMPL
PB124092BS - 1	LCSS	18870	3.3529	-7471B	PPB		18 Oct 2019 09:01:37	U	SMPL
K5153-01 - 1	TR-04-101619	1644	0.2564	-7471B	PPB		18 Oct 2019 09:03:54	U	SMPL
K5393-01 - 1	T-6-D1-D3-(0-46)	18690	3.3205	-7471B	PPB		18 Oct 2019 09:06:12	U	SMPL
K5393-08 - 1	T-9-U1-U3-(0-28)	10370	1.8249	-7471B	PPB		18 Oct 2019 09:08:29	U	SMPL
K5393-14 - 1	T-13-V1-(0-24)	3075	0.5136	-7471B	PPB		18 Oct 2019 09:10:57	U	SMPL
K5393-17 - 1	T-16-G1-(0-27)	31873	5.6902	-7471B	PPB		18 Oct 2019 09:13:13	U	SMPL
CCV68 - 1	CCV68	28763	5.1312	-7471B	PPB		18 Oct 2019 09:15:29	U	SMPL
CCB68 - 1	CCB68	48	-0.0305	-7471B	PPB		18 Oct 2019 09:17:44	U	SMPL
K5393-17DUP - 1	T-16-G1-(0-27)DUP	31324	5.5916	-7471B	PPB		18 Oct 2019 09:20:00	U	SMPL
K5393-17MSD - 1	T-16-G1-(0-27)MSD	49189	8.8029	-7471B	PPB		18 Oct 2019 09:24:33	U	SMPL
K5394-01 - 1	T-17-F1-(0-30)	94280	16.9083	-7471B	PPB		18 Oct 2019 09:26:50	U	SMPL
K5394-04 - 1	T-15-E1-(0-20)	6815	1.1859	-7471B	PPB		18 Oct 2019 09:29:08	U	SMPL
K5401-01 - 1	RBR200031-RT4221	2166	0.3502	-7471B	PPB		18 Oct 2019 09:31:27	U	SMPL
K5401-02 - 1	RBR200036-RT1488	3052	0.5095	-7471B	PPB		18 Oct 2019 09:33:44	U	SMPL
K5420-01 - 1	TP-1	301	0.0150	-7471B	PPB		18 Oct 2019 09:36:01	U	SMPL
K5420-03 - 1	TP-2	405	0.0337	-7471B	PPB		18 Oct 2019 09:38:19	U	SMPL
K5420-05 - 1	TP-3	447	0.0412	-7471B	PPB		18 Oct 2019 09:40:35	U	SMPL
CCV69 - 1	CCV69	28956	5.1659	-7471B	PPB		18 Oct 2019 09:42:52	U	SMPL
CCB69 - 1	CCB69	34	-0.0330	-7471B	PPB		18 Oct 2019 09:45:08	U	SMPL
K5420-07 - 1	TP-4	491	0.0491	-7471B	PPB		18 Oct 2019 09:47:24	U	SMPL
K5420-09 - 1	TP-5	381	0.0294	-7471B	PPB		18 Oct 2019 09:49:40	U	SMPL
K5420-11 - 1	TP-6	425	0.0373	-7471B	PPB		18 Oct 2019 09:51:56	U	SMPL
K5420-13 - 1	SP-1	4446	0.7601	-7471B	PPB		18 Oct 2019 09:54:13	U	SMPL
K5420-15 - 1	SP-2	4853	0.8332	-7471B	PPB		18 Oct 2019 09:56:30	U	SMPL
K5436-01 - 1	3425-28	3189	0.5341	-7471B	PPB		18 Oct 2019 09:58:46	U	SMPL
K5436-04 - 1	3860-50	3939	0.6689	-7471B	PPB		18 Oct 2019 10:01:04	U	SMPL
K5393-17LX5 - 1		5851	1.0126	-7471B	PPB		18 Oct 2019 10:03:21	U	SMPL
K5393-17MS - 1	T-16-G1-(0-27)MS	49618	8.8800	-7471B	PPB		18 Oct 2019 10:10:57	U	SMPL
CCV70 - 1	CCV70	28658	5.1123	-7471B	PPB		18 Oct 2019 10:13:14	U	SMPL
CCB70 - 1	CCB70	64	-0.0276	-7471B	PPB		18 Oct 2019 10:19:09	U	SMPL
K5394-01DLX4 - 1		24169	4.3054	-7471B	PPB		18 Oct 2019 10:21:25	U	SMPL
K5393-17A - 1		49320	8.8264	-7471B	PPB		18 Oct 2019 10:23:41	U	SMPL
CCV71 - 1	CCV71	29045	5.1819	-7471B	PPB		18 Oct 2019 10:25:57	U	SMPL
CCB71 - 1	CCB71	48	-0.0305	-7471B	PPB		18 Oct 2019 10:28:15	U	SMPL