

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CP

Instrument ID : Konelab

10/22/2019 13:21


Test Nitrite

Accepted 10/22/2019 13:21

Factor 0.401
Bias 0.008

Coeff. of det. 0.999657

Errors Meas. error

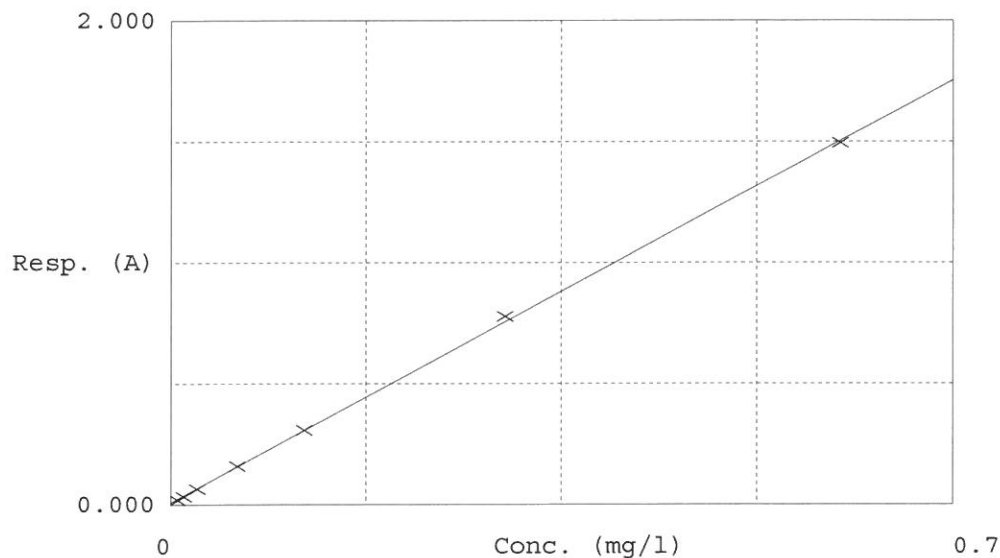

	Calibrator	Response	Calc. con.	Conc.	Errors
1	NITRITE0.6	0.018	0.0040	0.0060	Blank resp. low
2	NITRITE0.6	0.034	0.0104	0.0120	Blank resp. low
3	NITRITE0.6	0.065	0.0228	0.0240	
4	NITRITE0.6	0.159	0.0604	0.0600	
5	NITRITE0.6	0.308	0.1202	0.1200	
6	NITRITE0.6	0.778	0.3085	0.3000	
7	NITRITE0.6	1.494	0.5958	0.6000	Blank resp. low

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CS

Instrument ID : Konelab

10/22/2019 13:50

Test: Nitrite

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.307 ✓	0.0	0.774	Blank resp. low
ICB1	-0.002 ✓	0.0	0.004	Blank resp. low
CCV1	0.303 ✓	0.0	0.763	Blank resp. low
CCB1	-0.000 ✓	0.0	0.007	Blank resp. low
LB105855BL	-0.001 ✓	0.0	0.007	Blank resp. low
LB105855BS	0.314 ✓	0.0	0.790	Blank resp. low
K5111-09	0.001 ✓	0.0	0.009	Blank resp. low
CCV2	0.304 ✓	0.0	0.767	
CCB2	-0.000 ✓	0.0	0.007	

N	9
Mean	0.136
SD	0.1620
CV%	119.06

Aquakem v. 7.2AQ1

Results from time period:

Tue Oct 22 11:17:20 2019

Tue Oct 22 13:47:34 2019

CT
10/22/19

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0061PPM	A	Nitrite	P	0.004	mg/l	10/22/2019 13:17:37	
0.0122PPM	A	Nitrite	P	0.0104	mg/l	10/22/2019 13:17:38	
0.0243PPM	A	Nitrite	P	0.0228	mg/l	10/22/2019 13:17:39	
0.0608PPM	A	Nitrite	P	0.0604	mg/l	10/22/2019 13:17:40	
0.1216PPM	A	Nitrite	P	0.1202	mg/l	10/22/2019 13:17:41	
0.304PPM	A	Nitrite	P	0.3085	mg/l	10/22/2019 13:17:42	
0.608PPM	A	Nitrite	P	0.5958	mg/l	10/22/2019 13:17:43	
ICV1	S	Nitrite	P	0.3069	mg/l	10/22/2019 13:47:23	
ICB1	S	Nitrite	P	-0.0018	mg/l	10/22/2019 13:47:24	
CCV1	S	Nitrite	P	0.3027	mg/l	10/22/2019 13:47:25	
CCB1	S	Nitrite	P	-0.0005	mg/l	10/22/2019 13:47:26	
LB105855BL	S	Nitrite	P	-0.0006	mg/l	10/22/2019 13:47:27	
LB105855BS	S	Nitrite	P	0.3136	mg/l	10/22/2019 13:47:28	
K5111-09	S	Nitrite	P	0.0005	mg/l	10/22/2019 13:47:29	
CCV2	S	Nitrite	P	0.3041	mg/l	10/22/2019 13:47:32	
CCB2	S	Nitrite	P	-0.0003	mg/l	10/22/2019 13:47:33	