


LB105923

7471B

INSTRUMENT ID: CV1

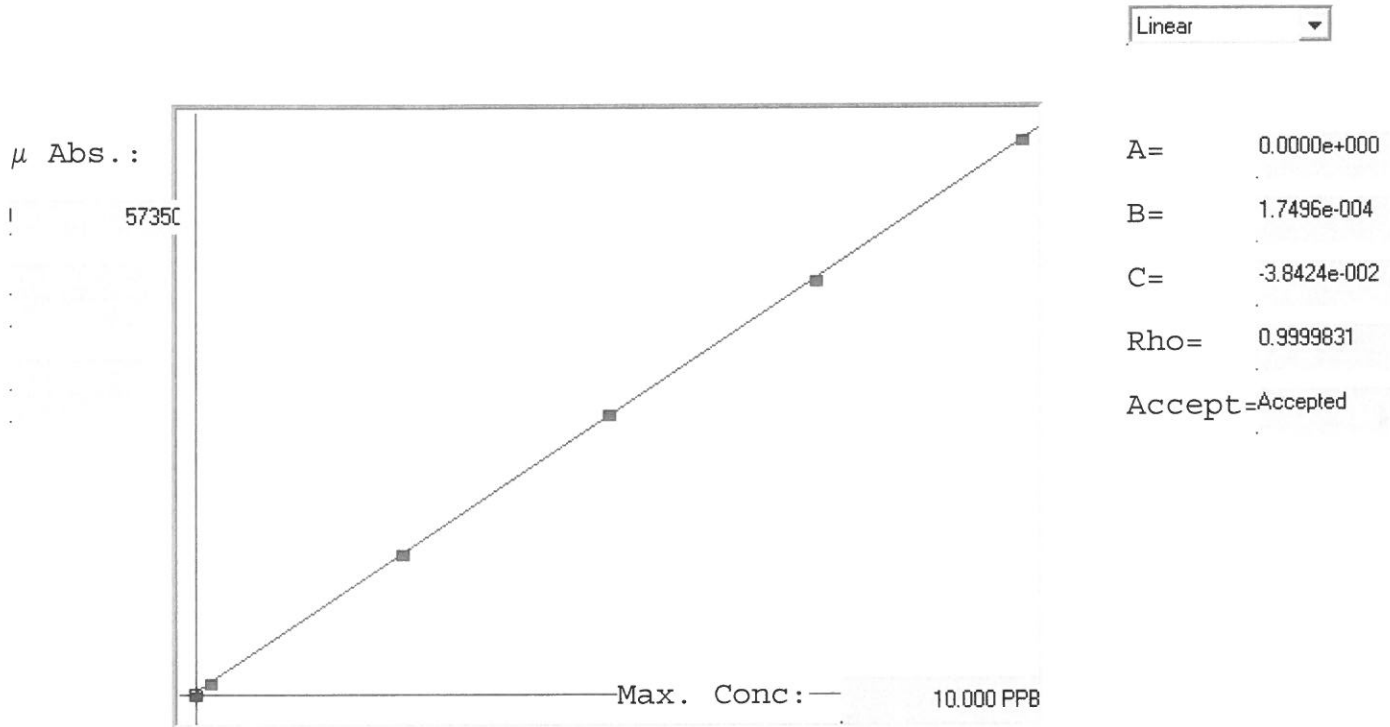

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.004	-0.004	195	0.000	195				
0.2	0.200	0.177	-0.023	1231	0.0 %	1231				
2.5	2.500	2.521	0.021	14631	0.0 %	14631				
5.0	5.000	5.034	0.034	28992	0.0 %	28992				
7.5	7.500	7.476	-0.024	42950	0.0 %	42950				
10.0	10.000	9.996	-0.004	57350	0.0 %	57350				

LB105923 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 25 Oct 2019 08:34:28					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	195	-	0.0000	7471B	PPB	25 Oct 2019 08:44:20	S	Std
0.2 - 1	50.2	1231	-	0.2000	7471B	PPB	25 Oct 2019 08:46:38	S	Std
2.5 - 1	52.5	14631	-	2.5000	7471B	PPB	25 Oct 2019 08:48:56	S	Std
5.0 - 1	55.6	28992	-	5.0000	7471B	PPB	25 Oct 2019 08:51:14	S	Std
7.5 - 1	57.5	42950	-	7.5000	7471B	PPB	25 Oct 2019 08:53:31	S	Std
10.0 - 1	510.0	57350	-	10.0000	7471B	PPB	25 Oct 2019 08:55:48	S	Std
ICV73 - 1	ICV73	23481	4.0699	-	7471B	PPB	25 Oct 2019 08:58:28	U	SMPL
ICB73 - 1	ICB73	115	-0.0183	-	7471B	PPB	25 Oct 2019 09:00:43	U	SMPL
CCV13 - 1	CCV13	28994	5.0344	-	7471B	PPB	25 Oct 2019 09:02:58	U	SMPL
CCB13 - 1	CCB13	116	-0.0181	-	7471B	PPB	25 Oct 2019 09:05:14	U	SMPL
CRA - 1	CRA	1248	0.1799	-	7471B	PPB	25 Oct 2019 09:07:29	U	SMPL
HighStd - 1	HighStd	58086	10.1244	-	7471B	PPB	25 Oct 2019 09:09:45	U	SMPL
ChkStd - 1	ChkStd	40224	6.9992	-	7471B	PPB	25 Oct 2019 09:12:01	U	SMPL
PB124294BL - 1	PBS	100	-0.0209	-	7471B	PPB	25 Oct 2019 09:14:17	U	SMPL
PB124294BS - 1	LCSS	22205	3.8466	-	7471B	PPB	25 Oct 2019 09:16:35	U	SMPL
K5145-04 - 1	HD-02-102319	1674	0.2545	-	7471B	PPB	25 Oct 2019 09:18:52	U	SMPL
K5148-09 - 1	OR-02-102319	2250	0.3552	-	7471B	PPB	25 Oct 2019 09:21:09	U	SMPL
K5153-05 - 1	TR-05-102419	4581	0.7631	-	7471B	PPB	25 Oct 2019 09:23:26	U	SMPL
K5512-01 - 1	CHRT-26706	950	0.1278	-	7471B	PPB	25 Oct 2019 09:25:44	U	SMPL
K5512-01DUP - 1	CHRT-26706DUP	948	0.1274	-	7471B	PPB	25 Oct 2019 09:28:00	U	SMPL
CCV14 - 1	CCV14	29140	5.0600	-	7471B	PPB	25 Oct 2019 09:30:16	U	SMPL
CCB14 - 1	CCB14	239	0.0034	-	7471B	PPB	25 Oct 2019 09:32:32	U	SMPL
K5512-01MS - 1	CHRT-26706MS	22617	3.9187	-	7471B	PPB	25 Oct 2019 09:34:48	U	SMPL
K5512-01MSD - 1	CHRT-26706MSD	22737	3.9397	-	7471B	PPB	25 Oct 2019 09:37:04	U	SMPL
K5533-01 - 1	P001-CHIP001-01	125609	21.9384	-	7471B	PPB	25 Oct 2019 09:39:21	U	SMPL
K5533-02 - 1	P001-CHIP002-01	36722	6.3865	-	7471B	PPB	25 Oct 2019 09:41:38	U	SMPL
K5543-01 - 1	R-1	410	0.0333	-	7471B	PPB	25 Oct 2019 09:43:57	U	SMPL
K5544-01 - 1	N-1	638	0.0732	-	7471B	PPB	25 Oct 2019 09:46:13	U	SMPL
K5545-01 - 1	C-1	665	0.0779	-	7471B	PPB	25 Oct 2019 09:48:31	U	SMPL
PB124299BL - 1	PBS	272	0.0092	-	7471B	PPB	25 Oct 2019 09:50:48	U	SMPL
PB124299BS - 1	LCSS	22343	3.8708	-	7471B	PPB	25 Oct 2019 09:53:06	U	SMPL
K5497-01 - 1	170-48-(0-1)	16894	2.9174	-	7471B	PPB	25 Oct 2019 09:55:22	U	SMPL
CCV15 - 1	CCV15	29143	5.0605	-	7471B	PPB	25 Oct 2019 09:57:38	U	SMPL
CCB15 - 1	CCB15	242	0.0039	-	7471B	PPB	25 Oct 2019 09:59:55	U	SMPL
K5497-03 - 1	169-90-(0-1.2)	4978	0.8325	-	7471B	PPB	25 Oct 2019 10:02:11	U	SMPL
K5497-05 - 1	169-32-(0-1)	4989	0.8345	-	7471B	PPB	25 Oct 2019 10:04:27	U	SMPL
K5497-05DUP - 1	169-32-(0-1)DUP	4996	0.8357	-	7471B	PPB	25 Oct 2019 10:06:43	U	SMPL
K5497-05MS - 1	169-32-(0-1)MS	23817	4.1286	-	7471B	PPB	25 Oct 2019 10:08:59	U	SMPL
K5497-05MSD - 1	169-32-(0-1)MSD	23467	4.0674	-	7471B	PPB	25 Oct 2019 10:11:15	U	SMPL
K5497-07 - 1	168-74-(0-1)	37303	6.4882	-	7471B	PPB	25 Oct 2019 10:13:32	U	SMPL
K5497-09 - 1	168-16-(0-1)	54519	9.5003	-	7471B	PPB	25 Oct 2019 10:15:49	U	SMPL
K5497-11 - 1	167-58-(0-1)	6835	1.1574	-	7471B	PPB	25 Oct 2019 10:18:07	U	SMPL
K5497-13 - 1	167-00-(0-1)	79583	13.8856	-	7471B	PPB	25 Oct 2019 10:20:26	U	SMPL
K5497-15 - 1	166-42-(0-1)	2525	0.4034	-	7471B	PPB	25 Oct 2019 10:22:42	U	SMPL
CCV16 - 1	CCV16	29516	5.1258	-	7471B	PPB	25 Oct 2019 10:25:00	U	SMPL
CCB16 - 1	CCB16	379	0.0279	-	7471B	PPB	25 Oct 2019 10:27:16	U	SMPL
K5497-17 - 1	188-46-(0-1)	1085	0.1514	-	7471B	PPB	25 Oct 2019 10:29:32	U	SMPL
K5497-19 - 1	189-04-(0-1.2)	3843	0.6340	-	7471B	PPB	25 Oct 2019 10:31:48	U	SMPL
K5498-01 - 1	189-62-(0-1)	2177	0.3425	-	7471B	PPB	25 Oct 2019 10:34:06	U	SMPL
K5498-03 - 1	190-20-(0-1)	16844	2.9086	-	7471B	PPB	25 Oct 2019 10:36:23	U	SMPL
K5498-05 - 1	190-78-(0-1)	10281	1.7604	-	7471B	PPB	25 Oct 2019 10:38:40	U	SMPL
K5498-07 - 1	196-00-(0-1)	22897	3.9677	-	7471B	PPB	25 Oct 2019 10:40:56	U	SMPL
K5498-09 - 1	196-58-(0-1)	12997	2.2356	-	7471B	PPB	25 Oct 2019 10:43:13	U	SMPL
K5498-11 - 1	191-36-(0-1)	33552	5.8319	-	7471B	PPB	25 Oct 2019 10:45:31	U	SMPL
K5498-13 - 1	191-94-(0-1)	32378	5.6265	-	7471B	PPB	25 Oct 2019 10:47:50	U	SMPL
K5498-15 - 1	191-52-(0-1)	42570	7.4097	-	7471B	PPB	25 Oct 2019 10:50:06	U	SMPL
CCV17 - 1	CCV17	29549	5.1315	-	7471B	PPB	25 Oct 2019 10:52:24	U	SMPL
CCB17 - 1	CCB17	468	0.0435	-	7471B	PPB	25 Oct 2019 10:54:42	U	SMPL
K5498-17 - 1	193-10-(0-1)	20075	3.4739	-	7471B	PPB	25 Oct 2019 10:56:59	U	SMPL
K5498-19 - 1	193-68-(0-1)	62186	10.8418	-	7471B	PPB	25 Oct 2019 10:59:17	U	SMPL
K5512-01LX5 - 1		320	0.0176	-	7471B	PPB	25 Oct 2019 11:01:34	U	SMPL
K5512-01A - 1		22776	3.9465	-	7471B	PPB	25 Oct 2019 11:03:53	U	SMPL
K5497-05LX5 - 1		1229	0.1766	-	7471B	PPB	25 Oct 2019 11:06:10	U	SMPL
K5497-05A - 1		23801	4.1258	-	7471B	PPB	25 Oct 2019 11:08:27	U	SMPL
K5533-01DLX5 - 1		24101	4.1783	-	7471B	PPB	25 Oct 2019 11:10:44	U	SMPL
K5497-13DLX3 - 1		23909	4.1447	-	7471B	PPB	25 Oct 2019 11:28:56	U	SMPL
K5498-19DLX2 - 1		31254	5.4298	-	7471B	PPB	25 Oct 2019 11:31:13	U	SMPL
CCV18 - 1	CCV18	29778	5.1716	-	7471B	PPB	25 Oct 2019 11:33:29	U	SMPL
CCB18 - 1	CCB18	375	0.0272	-	7471B	PPB	25 Oct 2019 11:35:46	U	SMPL