

LB105928

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CP

Instrument ID : Konelab

10/25/2019 10:13

Test Phenolics-


Accepted 10/25/2019 10:00

Factor 9.337

Bias 0.011

Coeff. of det. 0.999807


Errors

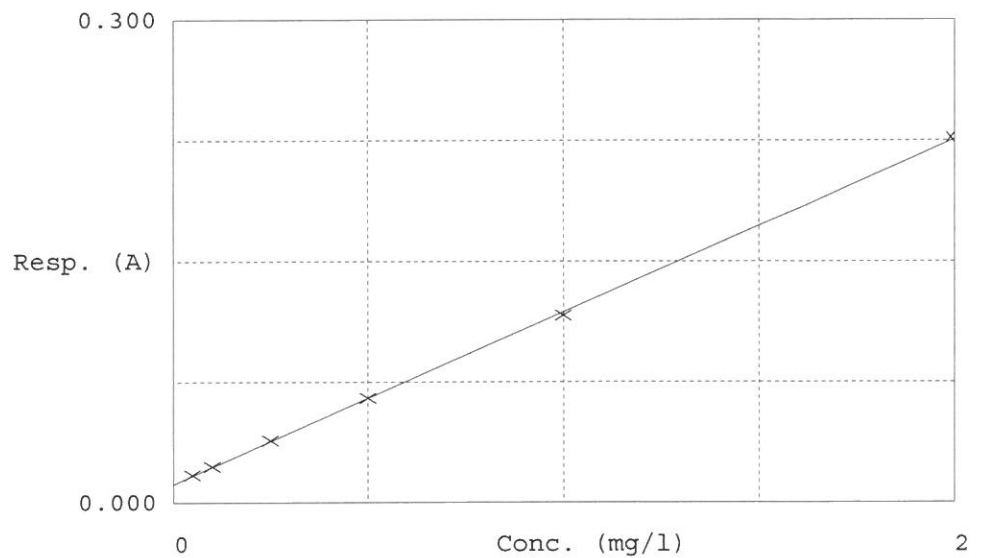

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.017	0.0542	0.0500	
2	Phenol-2	0.022	0.1024	0.1000	
3	Phenol-2	0.039	0.2540	0.2500	
4	Phenol-2	0.065	0.5004	0.5000	
5	Phenol-2	0.116	0.9797	1.0000	
6	Phenol-2	0.227	2.0093	2.0000	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by :



Instrument ID : Konelab

10/25/2019 10:35

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.991 ✓	0.0	0.118	
ICB1	0.004 ✓	0.0	0.012	
CCV1	0.967 ✓	0.0	0.115	
CCB1	0.016 ✓	0.0	0.013	
PB124231BL	0.015	0.0	0.013	
PB124231BS	0.994	0.0	0.118	
K5490-02	0.003	0.0	0.012	
K5490-02DUP	0.001	0.0	0.012	
K5490-02MS	0.991	0.0	0.118	
K5490-02MSD	0.988	0.0	0.117	
K5505-01	0.003	0.0	0.012	
CCV2	0.970 ✓	0.0	0.115	
CCB2	0.015 ✓	0.0	0.013	

N	13
Mean	0.458
SD	0.5062
CV%	110.44

Aquakem v. 7.2AQ1

Results from time period:

Fri Oct 25 09:59:24 2019

Fri Oct 25 10:34:13 2019

10/25/19

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0542	mg/l	10/25/2019 9:59:24	
0.1PPM	A	Phenolics-	P	0.1024	mg/l	10/25/2019 9:59:25	
0.25PPM	A	Phenolics-	P	0.254	mg/l	10/25/2019 9:59:26	
0.50PPM	A	Phenolics-	P	0.5004	mg/l	10/25/2019 9:59:27	
1.0PPM	A	Phenolics-	P	0.9797	mg/l	10/25/2019 9:59:28	
2.0PPM	A	Phenolics-	P	2.0093	mg/l	10/25/2019 9:59:29	
ICV1	S	Phenolics-	P	0.9913	mg/l	10/25/2019 10:29:45	
ICB1	S	Phenolics-	P	0.0044	mg/l	10/25/2019 10:29:46	
CCV1	S	Phenolics-	P	0.9671	mg/l	10/25/2019 10:29:47	
CCB1	S	Phenolics-	P	0.0162	mg/l	10/25/2019 10:29:48	
PB124231BL	S	Phenolics-	P	0.0153	mg/l	10/25/2019 10:29:49	
PB124231BS	S	Phenolics-	P	0.9939	mg/l	10/25/2019 10:29:50	
K5490-02	S	Phenolics-	P	0.0031	mg/l	10/25/2019 10:29:51	
K5490-02DUP	S	Phenolics-	P	0.001	mg/l	10/25/2019 10:29:52	
K5490-02MS	S	Phenolics-	P	0.9908	mg/l	10/25/2019 10:29:53	
K5490-02MSD	S	Phenolics-	P	0.9882	mg/l	10/25/2019 10:29:55	
K5505-01	S	Phenolics-	P	0.0027	mg/l	10/25/2019 10:34:11	
CCV2	S	Phenolics-	P	0.9705	mg/l	10/25/2019 10:34:12	
CCB2	S	Phenolics-	P	0.0146	mg/l	10/25/2019 10:34:13	