

LB105982 INSTRUMENT ID: CV1

Method: 245.1

Operator: Admin


Date of Analysis: 29 Oct 2019 12:00:37

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	67	-	0.0000	245.1	PPB	29 Oct 2019 12:03:59	S	Std
0.05 - 1	50-05	226	-	0.0500	245.1	PPB	29 Oct 2019 12:06:18	S	Std
0.2 - 1	50-2	715	-	0.2000	245.1	PPB	29 Oct 2019 12:08:36	S	Std
2.5 - 1	52-5	9042	-	2.5000	245.1	PPB	29 Oct 2019 12:10:54	S	Std
5.0 - 1	55-0	18548	-	5.0000	245.1	PPB	29 Oct 2019 12:13:11	S	Std
7.5 - 1	57-5	27376	-	7.5000	245.1	PPB	29 Oct 2019 12:15:28	S	Std
10.0 - 1	510-0	35938	-	10.0000	245.1	PPB	29 Oct 2019 12:26:31	S	Std
ICV78 - 1	ICV78	15191	4.1771	-245.1	PPB	PPB	29 Oct 2019 12:32:00	U	SMPL
ICB78 - 1	ICB78	-33	-0.0339	-245.1	PPB	PPB	29 Oct 2019 12:34:16	U	SMPL
CCV43 - 1	CCV43	19005	5.2321	-245.1	PPB	PPB	29 Oct 2019 12:36:31	U	SMPL
CCB43 - 1	CCB43	7	-0.0228	-245.1	PPB	PPB	29 Oct 2019 12:38:48	U	SMPL
CRA - 1	CRA	222	0.0367	-245.1	PPB	PPB	29 Oct 2019 12:51:35	U	SMPL
HighStd - 1	HighStd	35522	9.8007	-245.1	PPB	PPB	29 Oct 2019 12:53:50	U	SMPL
ChkStd - 1	ChkStd	25116	6.9224	-245.1	PPB	PPB	29 Oct 2019 12:56:07	U	SMPL
PB124395BL - 1	PBW	-17	-0.0294	-245.1	PPB	PPB	29 Oct 2019 12:58:24	U	SMPL
PB124395BS - 1	LCSW	16457	4.5273	-245.1	PPB	PPB	29 Oct 2019 13:00:42	U	SMPL
K5410-04 - 1	TI-604	76	-0.0037	-245.1	PPB	PPB	29 Oct 2019 13:03:00	U	SMPL
K5411-04 - 1	T1-658	146	0.0157	-245.1	PPB	PPB	29 Oct 2019 13:05:17	U	SMPL
K5505-01 - 1	55-ST-22	45	-0.0123	-245.1	PPB	PPB	29 Oct 2019 13:07:35	U	SMPL
K5505-01DUP - 1	55-ST-22DUP	52	-0.0103	-245.1	PPB	PPB	29 Oct 2019 13:09:53	U	SMPL
K5505-01MS - 1	55-ST-22MS	14057	3.8635	-245.1	PPB	PPB	29 Oct 2019 13:14:58	U	SMPL
CCV44 - 1	CCV44	18776	5.1688	-245.1	PPB	PPB	29 Oct 2019 13:17:14	U	SMPL
CCB44 - 1	CCB44	-5	-0.0261	-245.1	PPB	PPB	29 Oct 2019 13:19:31	U	SMPL
K5505-01MSD - 1	55-ST-22MSD	14021	3.8535	-245.1	PPB	PPB	29 Oct 2019 13:21:47	U	SMPL
K5582-02 - 1	NCQ-632	52	-0.0103	-245.1	PPB	PPB	29 Oct 2019 13:24:03	U	SMPL
K5583-06 - 1	OB-722	56	-0.0092	-245.1	PPB	PPB	29 Oct 2019 13:26:19	U	SMPL
K5505-01LX5 - 1		21	-0.0189	-245.1	PPB	PPB	29 Oct 2019 13:28:36	U	SMPL
K5505-01A - 1		14583	4.0090	-245.1	PPB	PPB	29 Oct 2019 13:30:52	U	SMPL
CCV45 - 1	CCV45	18833	5.1845	-245.1	PPB	PPB	29 Oct 2019 13:33:09	U	SMPL
CCB45 - 1	CCB45	13	-0.0211	-245.1	PPB	PPB	29 Oct 2019 13:35:27	U	SMPL

LB105982

245.1

INSTRUMENT ID : CV1

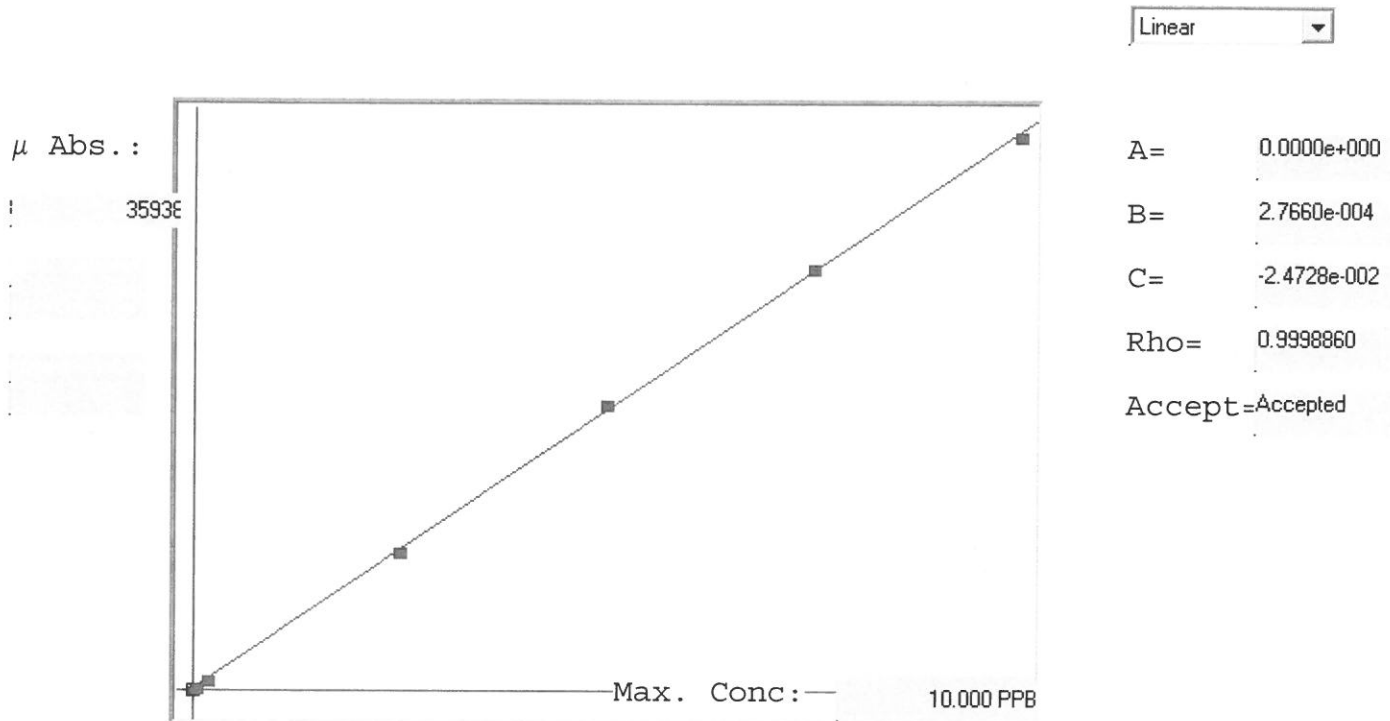

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.006	-0.006	67	0.000	67				
0.05	0.050	0.038	-0.012	226	0.0 %	226				
0.2	0.200	0.173	-0.027	715	0.0 %	715				
2.5	2.500	2.476	-0.024	9042	0.0 %	9042				
5.0	5.000	5.106	0.106	18548	0.0 %	18548				
7.5	7.500	7.548	0.048	27376	0.0 %	27376				
10.0	10.000	9.916	-0.084	35938	0.0 %	35938				