


LB105995

7470A

INSTRUMENT ID: CVI

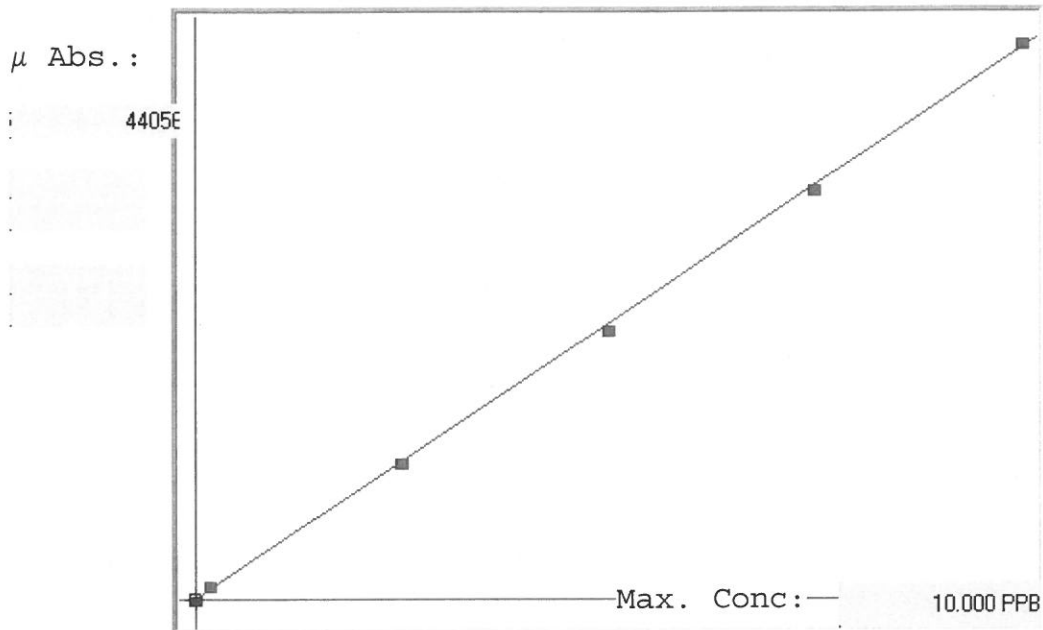

Linear

A= 0.0000e+000

B= 2.2861e-004

C= 6.1522e-003

Rho= 0.9998788

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.018	0.018	50	0.000	50				
0.2	0.200	0.255	0.055	1087	0.0 %	1087				
2.5	2.500	2.483	-0.017	10833	0.0 %	10833				
5.0	5.000	4.908	-0.092	21442	0.0 %	21442				
7.5	7.500	7.459	-0.041	32600	0.0 %	32600				
10.0	10.000	10.078	0.078	44056	0.0 %	44056				

LB105995 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 29 Oct 2019 14:17:48					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	50	-	0.0000	7470A	PPB	29 Oct 2019 14:21:52	S	Std
0.2 - 1	50.2	1087	-	0.2000	7470A	PPB	29 Oct 2019 14:24:01	S	Std
2.5 - 1	52.5	10833	-	2.5000	7470A	PPB	29 Oct 2019 14:26:10	S	Std
5.0 - 1	55.0	21442	-	5.0000	7470A	PPB	29 Oct 2019 14:28:19	S	Std
7.5 - 1	57.5	32600	-	7.5000	7470A	PPB	29 Oct 2019 14:30:27	S	Std
10.0 - 1	510.0	44056	-	10.0000	7470A	PPB	29 Oct 2019 14:46:08	S	Std
ICV79 - 1	ICV79	16628	3.8075	-	7470A	PPB	29 Oct 2019 14:49:04	U	SMPL
ICB79 - 1	ICB79	3	0.0068	-	7470A	PPB	29 Oct 2019 14:51:11	U	SMPL
CCV46 - 1	CCV46	21491	4.9193	-	7470A	PPB	29 Oct 2019 14:53:18	U	SMPL
CCB46 - 1	CCB46	27	0.0123	-	7470A	PPB	29 Oct 2019 14:55:24	U	SMPL
CRA - 1	CRA	1061	0.2487	-	7470A	PPB	29 Oct 2019 14:57:31	U	SMPL
HighStd - 1	HighStd	44026	10.0711	-	7470A	PPB	29 Oct 2019 14:59:37	U	SMPL
ChkStd - 1	ChkStd	29995	6.8634	-	7470A	PPB	29 Oct 2019 15:01:44	U	SMPL
PB124398BL - 1	PBW	-2	0.0057	-	7470A	PPB	29 Oct 2019 15:03:51	U	SMPL
PB124398BS - 1	LCSW	16884	3.8661	-	7470A	PPB	29 Oct 2019 15:05:59	U	SMPL
K5140-09 - 1	HR-06-102519	62	0.0203	-	7470A	PPB	29 Oct 2019 15:08:07	U	SMPL
K5140-09DUP - 1	HR-06-102519DUP	100	0.0290	-	7470A	PPB	29 Oct 2019 15:10:17	U	SMPL
K5140-09MS - 1	HR-06-102519MS	16577	3.7959	-	7470A	PPB	29 Oct 2019 15:12:39	U	SMPL
K5140-09MSD - 1	HR-06-102519MSD	17213	3.9413	-	7470A	PPB	29 Oct 2019 15:14:48	U	SMPL
K5564-03 - 1	CSA-2-1-1	77	0.0238	-	7470A	PPB	29 Oct 2019 15:16:54	U	SMPL
CCV47 - 1	CCV47	21572	4.9378	-	7470A	PPB	29 Oct 2019 15:19:01	U	SMPL
CCB47 - 1	CCB47	41	0.0155	-	7470A	PPB	29 Oct 2019 15:21:08	U	SMPL
K5564-06 - 1	CSA-2-1-2	106	0.0304	-	7470A	PPB	29 Oct 2019 15:23:16	U	SMPL
K5568-02 - 1	IDW-SOIL-102519	47	0.0169	-	7470A	PPB	29 Oct 2019 15:25:23	U	SMPL
PB124399BL - 1	PBW	26	0.0121	-	7470A	PPB	29 Oct 2019 15:27:30	U	SMPL
PB124399BS - 1	LCSW	16947	3.8805	-	7470A	PPB	29 Oct 2019 15:29:37	U	SMPL
K5569-02 - 1	IDW-DECON-WATER-102519	9880	2.2649	-	7470A	PPB	29 Oct 2019 15:31:45	U	SMPL
K5569-02DUP - 1	IDW-DECON-WATER-102519DUP	10111	2.3177	-	7470A	PPB	29 Oct 2019 15:33:53	U	SMPL
K5569-02MS - 1	IDW-DECON-WATER-102519MS	28063	6.4217	-	7470A	PPB	29 Oct 2019 15:36:01	U	SMPL
K5569-02MSD - 1	IDW-DECON-WATER-102519MSD	28866	6.6053	-	7470A	PPB	29 Oct 2019 15:38:09	U	SMPL
K5580-02 - 1	TT-007-IDWGW-20191025	120	0.0336	-	7470A	PPB	29 Oct 2019 15:40:18	U	SMPL
K5580-03 - 1	TT-008-IDWGW-20191025	93	0.0274	-	7470A	PPB	29 Oct 2019 15:42:24	U	SMPL
CCV48 - 1	CCV48	21485	4.9179	-	7470A	PPB	29 Oct 2019 15:44:31	U	SMPL
CCB48 - 1	CCB48	0	0.0062	-	7470A	PPB	29 Oct 2019 15:46:38	U	SMPL
PB124398TB - 1	PB124328TB	62	0.0203	-	7470A	PPB	29 Oct 2019 15:48:45	U	SMPL
K5140-09LX5 - 1		1	0.0064	-	7470A	PPB	29 Oct 2019 15:50:53	U	SMPL
K5140-09A - 1		17154	3.9278	-	7470A	PPB	29 Oct 2019 15:53:01	U	SMPL
K5569-02LX5 - 1		2051	0.4750	-	7470A	PPB	29 Oct 2019 15:55:12	U	SMPL
K5569-02A - 1		28644	6.5546	-	7470A	PPB	29 Oct 2019 15:57:20	U	SMPL
CCV49 - 1	CCV49	21656	4.9570	-	7470A	PPB	29 Oct 2019 15:59:28	U	SMPL
CCB49 - 1	CCB49	21	0.0110	-	7470A	PPB	29 Oct 2019 16:01:36	U	SMPL