


LB106193

7470A

INSTRUMENT ID :- CV1

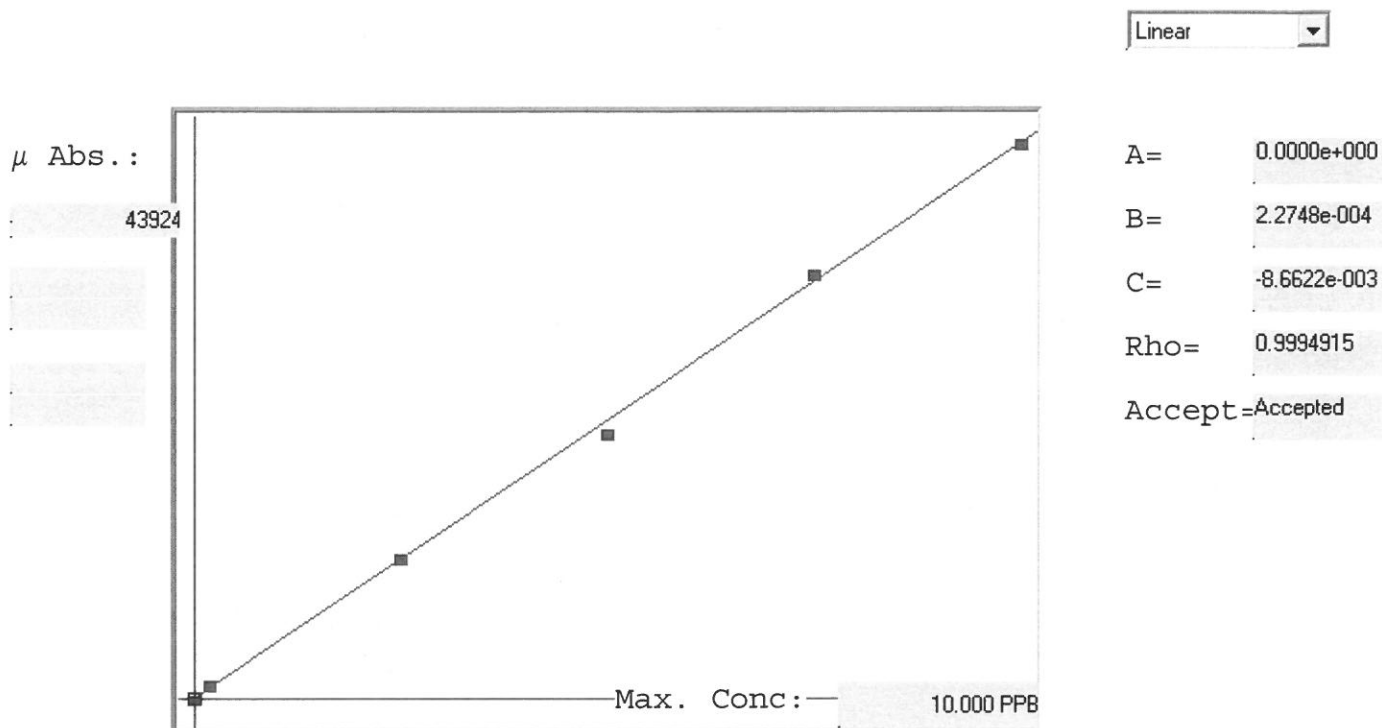

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.003	0.003	51	0.000	51				
0.2	0.200	0.256	0.056	1163	0.0 %	1163				
2.5	2.500	2.539	0.039	11200	0.0 %	11200				
5.0	5.000	4.766	-0.234	20990	0.0 %	20990				
7.5	7.500	7.653	0.153	33681	0.0 %	33681				
10.0	10.000	9.983	-0.017	43924	0.0 %	43924				

LB106193 INSTRUMENT ID CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 Nov 2019 11:50:56

Sample ID	Extended ID	μ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1		51	-	0.0000	7470A	PPB	11 Nov 2019 11:58:46	S	Std
0.2 - 1		1163	-	0.2000	7470A	PPB	11 Nov 2019 12:00:55	S	Std
2.5 - 1		11200	-	2.5000	7470A	PPB	11 Nov 2019 12:03:04	S	Std
5.0 - 1		20990	-	5.0000	7470A	PPB	11 Nov 2019 12:05:12	S	Std
7.5 - 1		33681	-	7.5000	7470A	PPB	11 Nov 2019 12:07:20	S	Std
10.0 - 1		43924	-	10.0000	7470A	PPB	11 Nov 2019 12:09:27	S	Std
ICV93 - 1	ICV93	18268	4.1469	-	7470A	PPB	11 Nov 2019 12:20:14	U	SMPL
ICB93 - 1	ICB93	-13	-0.0116	-	7470A	PPB	11 Nov 2019 12:22:20	U	SMPL
CCV15 - 1	CCV15	21706	4.9289	-	7470A	PPB	11 Nov 2019 12:24:26	U	SMPL
CCB15 - 1	CCB15	-25	-0.0143	-	7470A	PPB	11 Nov 2019 12:26:32	U	SMPL
CRA - 1	CRA	1131	0.2486	-	7470A	PPB	11 Nov 2019 12:28:38	U	SMPL
HighStd - 1	HighStd	43775	9.9491	-	7470A	PPB	11 Nov 2019 12:33:23	U	SMPL
ChkStd - 1	ChkStd	32382	7.3575	-	7470A	PPB	11 Nov 2019 12:40:14	U	SMPL
PB124684BL - 1	PBW	21	-0.0039	-	7470A	PPB	11 Nov 2019 12:42:21	U	SMPL
PB124684BS - 1	LCSW	17704	4.0186	-	7470A	PPB	11 Nov 2019 12:44:28	U	SMPL
K5673-08 - 1	PL-05-110819	-22	-0.0137	-	7470A	PPB	11 Nov 2019 12:46:35	U	SMPL
K5673-08DUP - 1	PL-05-110819DUP	7	-0.0071	-	7470A	PPB	11 Nov 2019 12:48:43	U	SMPL
K5673-08MS - 1	PL-05-110819MS	18479	4.1949	-	7470A	PPB	11 Nov 2019 12:50:50	U	SMPL
K5673-08MSD - 1	PL-05-110819MSD	18844	4.2779	-	7470A	PPB	11 Nov 2019 12:52:58	U	SMPL
K5676-15 - 1	SU-03-110819	-3	-0.0093	-	7470A	PPB	11 Nov 2019 12:55:05	U	SMPL
CCV16 - 1	CCV16	21314	4.8398	-	7470A	PPB	11 Nov 2019 12:57:11	U	SMPL
CCB16 - 1	CCB16	-16	-0.0123	-	7470A	PPB	11 Nov 2019 12:59:18	U	SMPL
K5746-07 - 1	TP-1A-COMP	11	-0.0062	-	7470A	PPB	11 Nov 2019 13:01:24	U	SMPL
K5758-02 - 1	CO-1008	9	-0.0066	-	7470A	PPB	11 Nov 2019 13:03:30	U	SMPL
K5760-03 - 1	RBR-50	20	-0.0041	-	7470A	PPB	11 Nov 2019 13:05:36	U	SMPL
K5760-08 - 1	3425	13	-0.0057	-	7470A	PPB	11 Nov 2019 13:07:43	U	SMPL
K5760-13 - 1	RBR-30	33	-0.0012	-	7470A	PPB	11 Nov 2019 13:09:50	U	SMPL
K5763-04 - 1	TP-37-S	26	-0.0027	-	7470A	PPB	11 Nov 2019 13:11:57	U	SMPL
K5763-08 - 1	TP-34-S	12	-0.0059	-	7470A	PPB	11 Nov 2019 13:14:05	U	SMPL
K5763-12 - 1	TP-34-D	26	-0.0027	-	7470A	PPB	11 Nov 2019 13:16:13	U	SMPL
K5771-02 - 1	SP	26	-0.0027	-	7470A	PPB	11 Nov 2019 13:18:21	U	SMPL
K5778-04 - 1	TP-33-S	11	-0.0062	-	7470A	PPB	11 Nov 2019 13:20:28	U	SMPL
CCV17 - 1	CCV17	21325	4.8423	-	7470A	PPB	11 Nov 2019 13:22:35	U	SMPL
CCB17 - 1	CCB17	48	0.0023	-	7470A	PPB	11 Nov 2019 13:24:41	U	SMPL
K5778-08 - 1	TP-35-S	1	-0.0084	-	7470A	PPB	11 Nov 2019 13:26:48	U	SMPL
PB124685BL - 1	PBW	17	-0.0048	-	7470A	PPB	11 Nov 2019 13:28:55	U	SMPL
PB124685BS - 1	LCSW	18279	4.1494	-	7470A	PPB	11 Nov 2019 13:31:01	U	SMPL
K5765-02 - 1	TT-009-IDWGW-20191107	366	0.0746	-	7470A	PPB	11 Nov 2019 13:33:08	U	SMPL
K5765-02DUP - 1	TT-009-IDWGW-20191107DUP	344	0.0696	-	7470A	PPB	11 Nov 2019 13:35:15	U	SMPL
K5765-02MS - 1	TT-009-IDWGW-20191107MS	19560	4.4408	-	7470A	PPB	11 Nov 2019 13:37:22	U	SMPL
K5765-02MSD - 1	TT-009-IDWGW-20191107MSD	18970	4.3066	-	7470A	PPB	11 Nov 2019 13:39:30	U	SMPL
K5765-03 - 1	TT-010-IDWGW-20191107	155	0.0266	-	7470A	PPB	11 Nov 2019 13:41:37	U	SMPL
K5765-04 - 1	TT-011-IDWGW-20191107	167	0.0293	-	7470A	PPB	11 Nov 2019 13:43:45	U	SMPL
K5777-07 - 1	AOC-7-MIDDLE	12717	2.8842	-	7470A	PPB	11 Nov 2019 13:45:52	U	SMPL
CCV18 - 1	CCV18	21109	4.7931	-	7470A	PPB	11 Nov 2019 13:47:59	U	SMPL
CCB18 - 1	CCB18	18	-0.0046	-	7470A	PPB	11 Nov 2019 13:50:05	U	SMPL
K5777-08 - 1	AOC-7-NORTH	22882	5.1965	-	7470A	PPB	11 Nov 2019 13:52:12	U	SMPL
PB124684TB - 1	PB124649TB	-16	-0.0123	-	7470A	PPB	11 Nov 2019 13:54:19	U	SMPL
K5673-08LX5 - 1		-2	-0.0091	-	7470A	PPB	11 Nov 2019 13:56:26	U	SMPL
K5673-08A - 1		18631	4.2295	-	7470A	PPB	11 Nov 2019 13:58:32	U	SMPL
K5765-02LX5 - 1		17	-0.0048	-	7470A	PPB	11 Nov 2019 14:00:39	U	SMPL
K5765-02A - 1		19262	4.3730	-	7470A	PPB	11 Nov 2019 14:02:46	U	SMPL
CCV19 - 1	CCV19	21429	4.8659	-	7470A	PPB	11 Nov 2019 14:04:55	U	SMPL
CCB19 - 1	CCB19	54	0.0036	-	7470A	PPB	11 Nov 2019 14:07:02	U	SMPL