


LB106199

INSTRUMENT ID: CV1

245.1

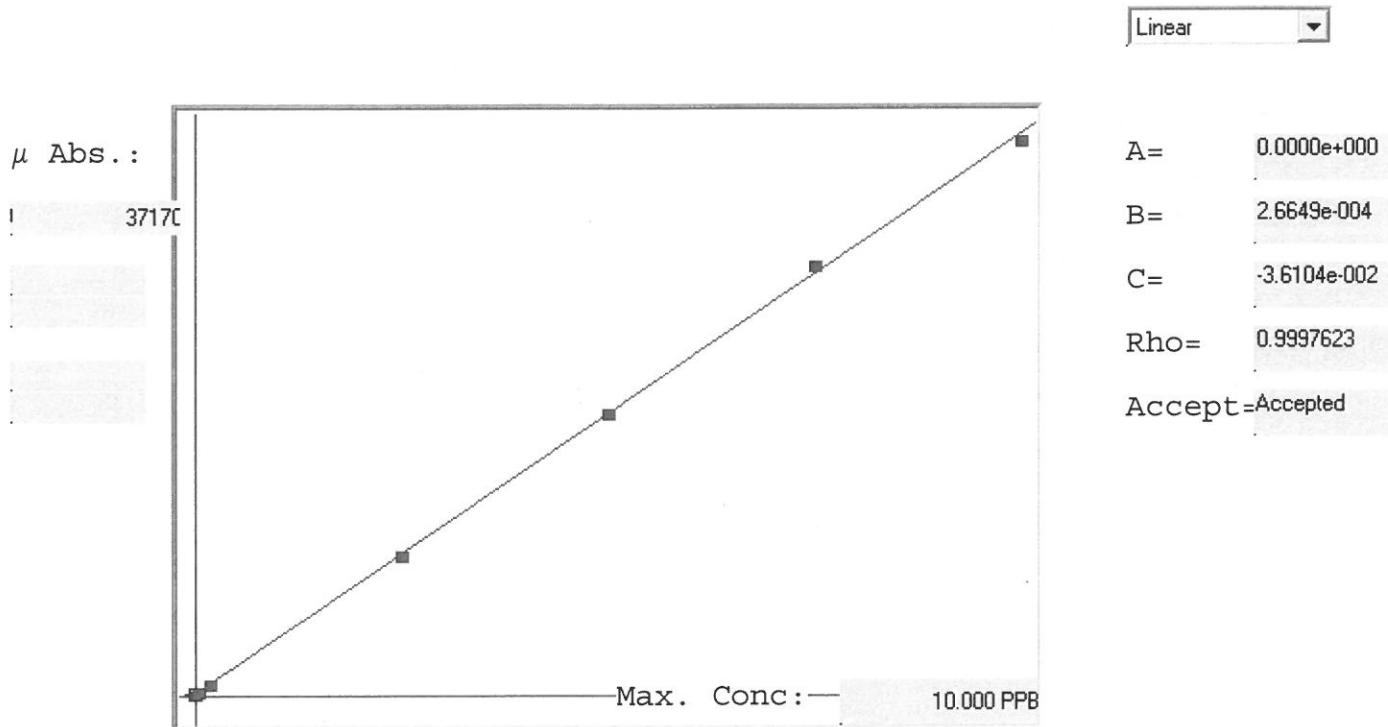

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.001	0.001	140	0.000	140				
0.05	0.050	0.045	-0.005	305	0.0 %	305				
0.2	0.200	0.173	-0.027	784	0.0 %	784				
2.5	2.500	2.482	-0.018	9448	0.0 %	9448				
5.0	5.000	5.014	0.014	18952	0.0 %	18952				
7.5	7.500	7.666	0.166	28901	0.0 %	28901				
10.0	10.000	9.869	-0.131	37170	0.0 %	37170				

LB106199 INSTRUMENT ID CV1

Method: 245.1

Operator: Admin

Date of Analysis: 11 Nov 2019 14:52:16

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	S 0.0	140	-	0.0000	245.1	PPB	11 Nov 2019 14:57:10	S	Std
0.05 - 1	S 0.05	305	-	0.0500	245.1	PPB	11 Nov 2019 14:59:27	S	Std
0.2 - 1	S 0.2	784	-	0.2000	245.1	PPB	11 Nov 2019 15:01:45	S	Std
2.5 - 1	S 2.5	9448	-	2.5000	245.1	PPB	11 Nov 2019 15:04:02	S	Std
5.0 - 1	S 5.0	18952	-	5.0000	245.1	PPB	11 Nov 2019 15:06:20	S	Std
7.5 - 1	S 7.5	28901	-	7.5000	245.1	PPB	11 Nov 2019 15:08:36	S	Std
10.0 - 1	S 10.0	37170	-	10.0000	245.1	PPB	11 Nov 2019 15:10:52	S	Std
ICV94 - 1	ICV94	15482	4.0896	-245.1		PPB	11 Nov 2019 15:16:29	U	SMPL
ICB94 - 1	ICB94	92	-0.0116	-245.1		PPB	11 Nov 2019 15:18:44	U	SMPL
CCV20 - 1	CCV20	18949	5.0135	-245.1		PPB	11 Nov 2019 15:21:00	U	SMPL
CCB20 - 1	CCB20	106	-0.0079	-245.1		PPB	11 Nov 2019 15:23:15	U	SMPL
CRA - 1	CRA	303	0.0446	-245.1		PPB	11 Nov 2019 15:25:30	U	SMPL
HighStd - 1	HighStd	36747	9.7565	-245.1		PPB	11 Nov 2019 15:27:45	U	SMPL
ChkStd - 1	ChkStd	26038	6.9027	-245.1		PPB	11 Nov 2019 15:30:01	U	SMPL
PB124702BL - 1	PBW	101	-0.0092	-245.1		PPB	11 Nov 2019 15:32:19	U	SMPL
PB124702BS - 1	LCSW	16473	4.3537	-245.1		PPB	11 Nov 2019 15:37:55	U	SMPL
K5709-02 - 1	COMP	806	0.1787	-245.1		PPB	11 Nov 2019 15:40:12	U	SMPL
K5709-02DUP - 1	COMPDUP	666	0.1414	-245.1		PPB	11 Nov 2019 15:42:29	U	SMPL
K5709-02MS - 1	COMPMS	13557	3.5766	-245.1		PPB	11 Nov 2019 15:44:46	U	SMPL
K5709-02MSD - 1	COMPMSD	13179	3.4759	-245.1		PPB	11 Nov 2019 15:47:03	U	SMPL
K5762-01 - 1	HP-640	73	-0.0167	-245.1		PPB	11 Nov 2019 15:49:21	U	SMPL
CCV21 - 1	CCV21	18856	4.9888	-245.1		PPB	11 Nov 2019 15:51:40	U	SMPL
CCB21 - 1	CCB21	75	-0.0161	-245.1		PPB	11 Nov 2019 15:53:56	U	SMPL
K5709-02LX5 - 1		159	0.0063	-245.1		PPB	11 Nov 2019 15:56:12	U	SMPL
K5709-02A - 1		15297	4.0403	-245.1		PPB	11 Nov 2019 15:58:27	U	SMPL
CCV22 - 1	CCV22	18342	4.8518	-245.1		PPB	11 Nov 2019 16:00:43	U	SMPL
CCB22 - 1	CCB22	140	0.0012	-245.1		PPB	11 Nov 2019 16:03:00	U	SMPL