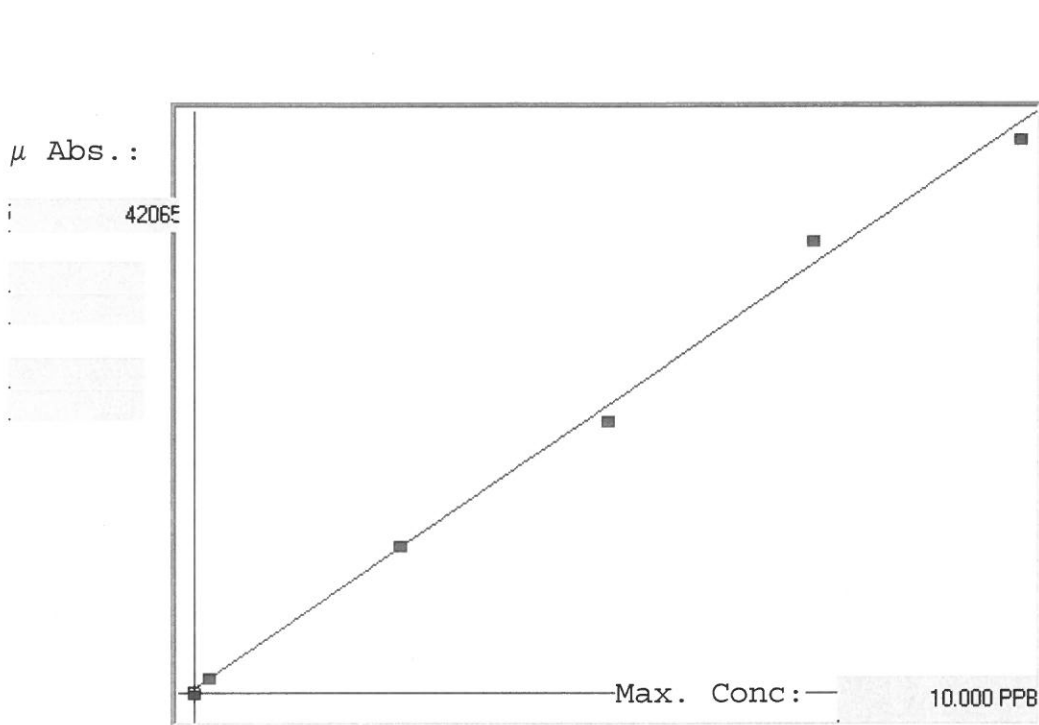


LB106255

ISM02.4

INSTRUMENT ID - CVA
MDL - Water ISM02.4 - 2019

Linear

A= 0.0000e+000

B= 2.3260e-004

C= -6.0078e-002

Rho= 0.9979773

Accept=Accepted

slope
y intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	2-1.
0.00	0.000	-0.036	-0.036	105	0.000	105					
0.05	0.050										
0.20	0.200	0.216	0.016	1186	0.0 %	1186					8%.
2.50	2.500	2.569	0.069	11301	0.0 %	11301					3%.
5.00	5.000	4.780	-0.220	20809	0.0 %	20809					-4%.
7.50	7.500	7.947	0.447	34423	0.0 %	34423					6%.
10.0	10.000	9.724	-0.276	42065	0.0 %	42065					-3%.

LB106255
INSTRUMENT ID CV1

Sample ID	Extended II μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
0 S0	117	-	0	ISM02.4	PPB	11/13/2019 13:56	Std
0.2 S0.2	362	-	0.2	ISM02.4	PPB	11/13/2019 13:58	Std
2.5 S2.5	3713	-	2.5	ISM02.4	PPB	11/13/2019 14:00	Std
5 S5	20809	-	5	ISM02.4	PPB	11/13/2019 14:28	Std
7.5 S7.5	34423	-	7.5	ISM02.4	PPB	11/13/2019 14:31	Std
10 S10	42065	-	10	ISM02.4	PPB	11/13/2019 14:33	Std
ICV	ICV	18010	4.1291	-	ISM02.4	PPB	11/13/2019 14:50 SMPL
ICB	ICB	88	-0.0396	-	ISM02.4	PPB	11/13/2019 14:52 SMPL
CCV041	CCV041	21025	4.8304	-	ISM02.4	PPB	11/13/2019 14:54 SMPL
CCB041	CCB041	72	-0.0433	-	ISM02.4	PPB	11/13/2019 14:57 SMPL
PB124740BL	PBW740	129	-0.0301	-	ISM02.4	PPB	11/13/2019 14:59 SMPL
K5695-08	MDL-WATE	503	0.0569	-	ISM02.4	PPB	11/13/2019 15:01 SMPL
K5695-09	MDL-WATE	505	0.0574	-	ISM02.4	PPB	11/13/2019 15:03 SMPL
K5695-10	MDL-WATE	505	0.0574	-	ISM02.4	PPB	11/13/2019 15:06 SMPL
K5695-11	MDL-WATE	515	0.0597	-	ISM02.4	PPB	11/13/2019 15:08 SMPL
K5695-12	MDL-WATE	504	0.0572	-	ISM02.4	PPB	11/13/2019 15:23 SMPL
K5695-13	MDL-WATE	480	0.0516	-	ISM02.4	PPB	11/13/2019 15:25 SMPL
K5695-14	MDL-WATE	493	0.0546	-	ISM02.4	PPB	11/13/2019 15:28 SMPL
CCV042	CCV042	20958	4.8148	-	ISM02.4	PPB	11/13/2019 15:30 SMPL
CCB042	CCB042	104	-0.0359	-	ISM02.4	PPB	11/13/2019 15:37 SMPL