


7470A

LB 106280
INSTRUMENT ID: CV1

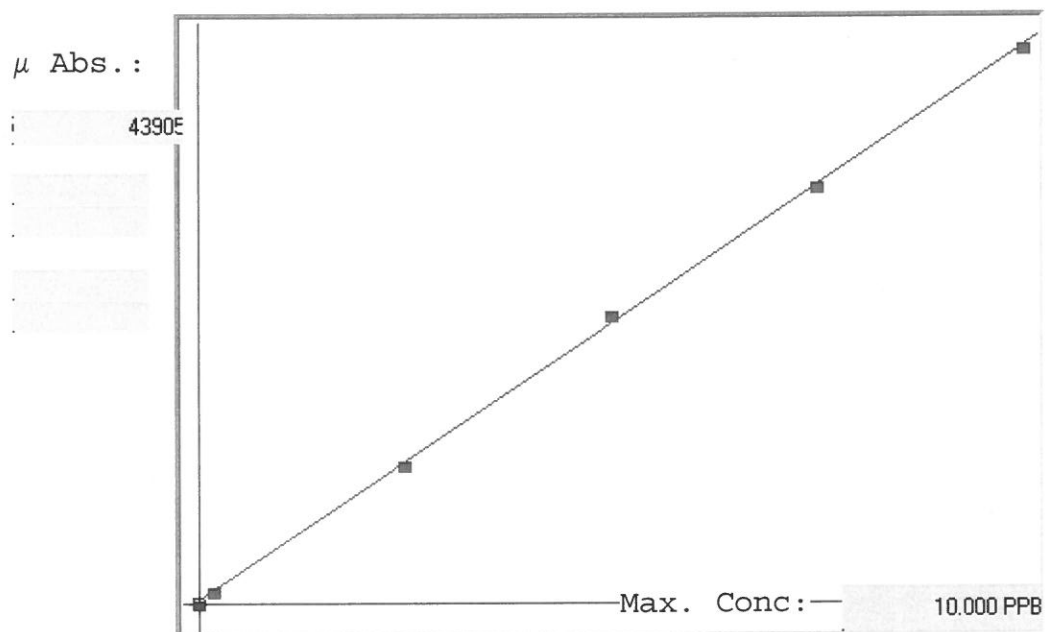

Linear

A= 0.0000e+000

B= 2.2751e-004

C= -4.6724e-002

Rho= 0.9998111

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.034	-0.034	56	0.000	56				
0.2	0.200	0.181	-0.019	1003	0.0 %	1003				
2.5	2.500	2.476	-0.024	11090	0.0 %	11090				
5.0	5.000	5.158	0.158	22876	0.0 %	22876				
7.5	7.500	7.476	-0.024	33067	0.0 %	33067				
10.0	10.000	9.942	-0.058	43905	0.0 %	43905				

LB106280 INSTRUMENT ID CV1

Method: 7470A		Operator: Admin		Date of Analysis: 14 Nov 2019 13:34:16					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	56	-	0.0000	7470A	PPB	14 Nov 2019 13:36:15	S	Std
0.2 - 1	50.2	1003	-	0.2000	7470A	PPB	14 Nov 2019 13:38:24	S	Std
2.5 - 1	52.5	11090	-	2.5000	7470A	PPB	14 Nov 2019 13:40:34	S	Std
5.0 - 1	55.0	22876	-	5.0000	7470A	PPB	14 Nov 2019 13:42:42	S	Std
7.5 - 1	57.5	33067	-	7.5000	7470A	PPB	14 Nov 2019 13:44:51	S	Std
10.0 - 1	510.0	43905	-	10.0000	7470A	PPB	14 Nov 2019 13:46:59	S	Std
ICV05 - 1	ICV05	16479	3.7024		7470A	PPB	14 Nov 2019 13:54:46	U	SMPL
ICB05 - 1	ICB05	-3	-0.0474		7470A	PPB	14 Nov 2019 13:56:52	U	SMPL
CCV49 - 1	CCV49	23200	5.2315		7470A	PPB	14 Nov 2019 13:59:00	U	SMPL
CCB49 - 1	CCB49	-6	-0.0481		7470A	PPB	14 Nov 2019 14:01:07	U	SMPL
CRA - 1	CRA	998	0.1803		7470A	PPB	14 Nov 2019 14:03:14	U	SMPL
HighStd - 1	HighStd	44327	10.0381		7470A	PPB	14 Nov 2019 14:05:20	U	SMPL
ChkStd - 1	ChkStd	31162	7.0429		7470A	PPB	14 Nov 2019 14:07:27	U	SMPL
PB124809BL - 1	PBW	-22	-0.0517		7470A	PPB	14 Nov 2019 14:09:35	U	SMPL
PB124809BS - 1	LCSW	16696	3.7518		7470A	PPB	14 Nov 2019 14:11:43	U	SMPL
K5822-01 - 1	N35868	1530	0.3014		7470A	PPB	14 Nov 2019 14:13:51	U	SMPL
K5822-01DUP - 1	N35868DUP	1526	0.3005		7470A	PPB	14 Nov 2019 14:15:59	U	SMPL
K5822-01MS - 1	N35868MS	19176	4.3160		7470A	PPB	14 Nov 2019 14:18:07	U	SMPL
K5822-01MSD - 1	N35868MSD	19104	4.2996		7470A	PPB	14 Nov 2019 14:20:16	U	SMPL
PB124810BL - 1	PBW	3	-0.0460		7470A	PPB	14 Nov 2019 14:22:23	U	SMPL
CCV50 - 1	CCV50	23051	5.1976		7470A	PPB	14 Nov 2019 14:24:29	U	SMPL
CCB50 - 1	CCB50	5	-0.0456		7470A	PPB	14 Nov 2019 14:26:37	U	SMPL
PB124810BS - 1	LCSW	16411	3.6869		7470A	PPB	14 Nov 2019 14:28:43	U	SMPL
K5668-07 - 1	HD-02-111319	13	-0.0438		7470A	PPB	14 Nov 2019 14:30:51	U	SMPL
K5670-08 - 1	OK-03-111219	41	-0.0374		7470A	PPB	14 Nov 2019 14:32:58	U	SMPL
K5813-02 - 1	SP-B	433	0.0518		7470A	PPB	14 Nov 2019 14:35:05	U	SMPL
K5826-04 - 1	TP-15-S	36	-0.0385		7470A	PPB	14 Nov 2019 14:37:12	U	SMPL
K5826-08 - 1	TP-14B-S	41	-0.0374		7470A	PPB	14 Nov 2019 14:39:20	U	SMPL
K5826-08DUP - 1	TP-14B-SDUP	44	-0.0367		7470A	PPB	14 Nov 2019 14:41:28	U	SMPL
K5826-08MS - 1	TP-14B-SMS	15796	3.5470		7470A	PPB	14 Nov 2019 14:43:37	U	SMPL
K5826-08MSD - 1	TP-14B-SMSD	16068	3.6089		7470A	PPB	14 Nov 2019 14:45:46	U	SMPL
K5822-01LX5 - 1		329	0.0281		7470A	PPB	14 Nov 2019 14:47:53	U	SMPL
CCV51 - 1	CCV51	22982	5.1819		7470A	PPB	14 Nov 2019 14:50:00	U	SMPL
CCB51 - 1	CCB51	8	-0.0449		7470A	PPB	14 Nov 2019 14:52:06	U	SMPL
K5826-08LX5 - 1		0	-0.0467		7470A	PPB	14 Nov 2019 14:54:14	U	SMPL
PB124810TB - 1	PB124762TB	127	-0.0178		7470A	PPB	14 Nov 2019 14:56:20	U	SMPL
CCV52 - 1	CCV52	23172	5.2251		7470A	PPB	14 Nov 2019 14:58:27	U	SMPL
CCB52 - 1	CCB52	-1	-0.0470		7470A	PPB	14 Nov 2019 15:00:35	U	SMPL