


LB106337

INSTRUMENT ID CVI

7470A

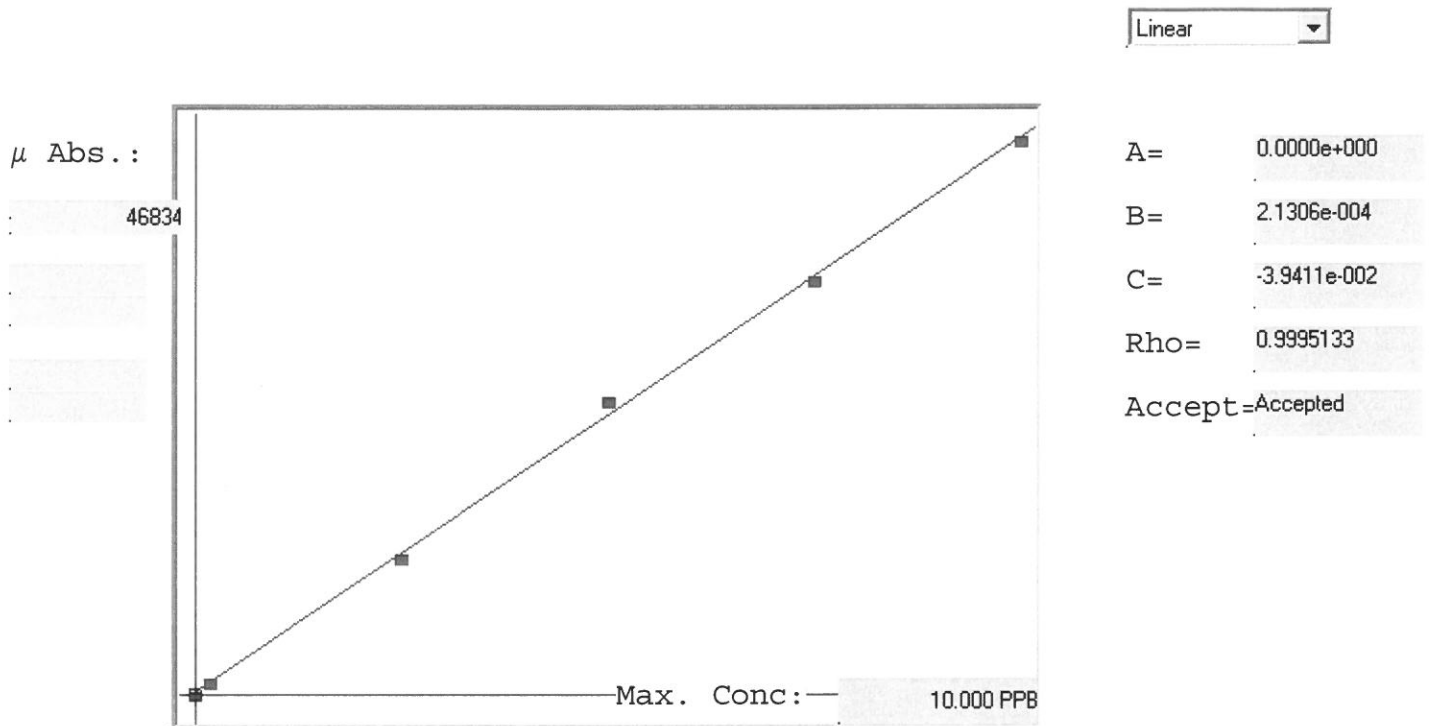

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.023	-0.023	78	0.000	78				
0.2	0.200	0.170	-0.030	984	0.0 %	984				
2.5	2.500	2.436	-0.064	11619	0.0 %	11619				
5.0	5.000	5.254	0.254	24844	0.0 %	24844				
7.5	7.500	7.423	-0.077	35027	0.0 %	35027				
10.0	10.000	9.939	-0.061	46834	0.0 %	46834				

LB106337 INSTRUMENT ID CV1

Method: 7470A		Operator: Admin		Date of Analysis: 16 Nov 2019 11:04:38					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1		78	-	0.0000	7470A	PPB	16 Nov 2019 11:09:36	S	Std
0.2 - 1		984	-	0.2000	7470A	PPB	16 Nov 2019 11:11:42	S	Std
2.5 - 1		11619	-	2.5000	7470A	PPB	16 Nov 2019 11:13:48	S	Std
5.0 - 1		24844	-	5.0000	7470A	PPB	16 Nov 2019 11:15:54	S	Std
7.5 - 1		35027	-	7.5000	7470A	PPB	16 Nov 2019 11:18:02	S	Std
10.0 - 1		46834	-	10.0000	7470A	PPB	16 Nov 2019 11:20:08	S	Std
ICV08 - 1	ICV08	18431	3.8875	-	7470A	PPB	16 Nov 2019 11:28:13	U	SMPL
ICB08 - 1	ICB08	-16	-0.0428	-	7470A	PPB	16 Nov 2019 11:30:19	U	SMPL
CCV64 - 1	CCV64	22156	4.6812	-	7470A	PPB	16 Nov 2019 11:32:25	U	SMPL
CCB64 - 1	CCB64	-11	-0.0418	-	7470A	PPB	16 Nov 2019 11:34:31	U	SMPL
CRA - 1	CRA	1007	0.1751	-	7470A	PPB	16 Nov 2019 11:36:37	U	SMPL
HighStd - 1	HighStd	46911	9.9555	-	7470A	PPB	16 Nov 2019 11:38:44	U	SMPL
ChkStd - 1	ChkStd	32069	6.7932	-	7470A	PPB	16 Nov 2019 11:40:50	U	SMPL
PB124864BL - 1	PBW	11	-0.0371	-	7470A	PPB	16 Nov 2019 11:42:56	U	SMPL
K5665-04 - 1	HR-05-111419	17	-0.0358	-	7470A	PPB	16 Nov 2019 11:47:11	U	SMPL
K5665-04DUP - 1	HR-05-111419DUP	8	-0.0377	-	7470A	PPB	16 Nov 2019 11:49:19	U	SMPL
K5665-04MS - 1	HR-05-111419MS	16566	3.4902	-	7470A	PPB	16 Nov 2019 11:55:09	U	SMPL
K5665-04MSD - 1	HR-05-111419MSD	16576	3.4923	-	7470A	PPB	16 Nov 2019 11:57:17	U	SMPL
K5671-10 - 1	OR-03-111419	-31	-0.0460	-	7470A	PPB	16 Nov 2019 11:59:23	U	SMPL
CCV65 - 1	CCV65	21516	4.5448	-	7470A	PPB	16 Nov 2019 12:01:29	U	SMPL
CCB65 - 1	CCB65	-45	-0.0490	-	7470A	PPB	16 Nov 2019 12:03:36	U	SMPL
K5782-08 - 1	TP-2A-COMP	29	-0.0332	-	7470A	PPB	16 Nov 2019 12:05:42	U	SMPL
K5807-02 - 1	P001-CC01-191111-01	21	-0.0349	-	7470A	PPB	16 Nov 2019 12:07:48	U	SMPL
K5807-04 - 1	P001-CC02-191111-01	38	-0.0313	-	7470A	PPB	16 Nov 2019 12:09:54	U	SMPL
K5807-06 - 1	P001-CC03-191111-01	204	0.0041	-	7470A	PPB	16 Nov 2019 12:12:01	U	SMPL
K5807-08 - 1	P001-CC04-191111-01	22	-0.0347	-	7470A	PPB	16 Nov 2019 12:14:07	U	SMPL
K5807-10 - 1	P001-CC05-191111-01	24	-0.0343	-	7470A	PPB	16 Nov 2019 12:16:14	U	SMPL
K5807-12 - 1	P001-CC06-191111-01	232	0.0100	-	7470A	PPB	16 Nov 2019 12:18:22	U	SMPL
K5807-14 - 1	P001-CC07-191111-01	48	-0.0292	-	7470A	PPB	16 Nov 2019 12:20:30	U	SMPL
K5807-16 - 1	P001-CC08-191112-01	-29	-0.0456	-	7470A	PPB	16 Nov 2019 12:22:38	U	SMPL
K5807-18 - 1	P001-CC09-191112-01	88	-0.0207	-	7470A	PPB	16 Nov 2019 12:24:44	U	SMPL
CCV66 - 1	CCV66	24856	5.2564	-	7470A	PPB	16 Nov 2019 12:28:21	U	SMPL
CCB66 - 1	CCB66	-12	-0.0420	-	7470A	PPB	16 Nov 2019 12:40:27	U	SMPL
K5807-20 - 1	P001-CC10-191112-01	51	-0.0285	-	7470A	PPB	16 Nov 2019 12:42:33	U	SMPL
K5838-03 - 1	UC-TP	5	-0.0383	-	7470A	PPB	16 Nov 2019 12:44:40	U	SMPL
K5848-01 - 1	ESW	30	-0.0330	-	7470A	PPB	16 Nov 2019 12:46:46	U	SMPL
K5858-02 - 1	DRUM-A	5	-0.0383	-	7470A	PPB	16 Nov 2019 12:48:52	U	SMPL
K5858-04 - 1	DRUM-B	19	-0.0354	-	7470A	PPB	16 Nov 2019 12:50:59	U	SMPL
K5862-04 - 1	TP-13A-S	21	-0.0349	-	7470A	PPB	16 Nov 2019 12:53:06	U	SMPL
K5863-07 - 1	TP-1-COMP	36	-0.0317	-	7470A	PPB	16 Nov 2019 12:55:14	U	SMPL
PB124867BL - 1	PBW	7	-0.0379	-	7470A	PPB	16 Nov 2019 12:57:22	U	SMPL
PB124867BS - 1	LCSW	19105	4.0311	-	7470A	PPB	16 Nov 2019 13:06:44	U	SMPL
K5807-22 - 1	P001-CC11-191112-01	-7	-0.0409	-	7470A	PPB	16 Nov 2019 13:08:50	U	SMPL
CCV67 - 1	CCV67	23798	5.0310	-	7470A	PPB	16 Nov 2019 13:14:31	U	SMPL
CCB67 - 1	CCB67	29	-0.0332	-	7470A	PPB	16 Nov 2019 13:16:37	U	SMPL
K5807-22DUP - 1	P001-CC11-191112-01DUP	13	-0.0366	-	7470A	PPB	16 Nov 2019 13:18:43	U	SMPL
K5807-22MS - 1	P001-CC11-191112-01MS	16766	3.5328	-	7470A	PPB	16 Nov 2019 13:20:49	U	SMPL
K5807-22MSD - 1	P001-CC11-191112-01MSD	16755	3.5304	-	7470A	PPB	16 Nov 2019 13:22:56	U	SMPL
K5807-24 - 1	P001-CC12-191112-01	-17	-0.0430	-	7470A	PPB	16 Nov 2019 13:25:02	U	SMPL
K5807-25 - 1	P001-CC13-191112-01	4	-0.0386	-	7470A	PPB	16 Nov 2019 13:27:09	U	SMPL
PB124887BL - 1	PBW	59	-0.0268	-	7470A	PPB	16 Nov 2019 13:29:16	U	SMPL
PB124887BS - 1	LCSW	18870	3.9810	-	7470A	PPB	16 Nov 2019 13:31:24	U	SMPL
K5822-02 - 1	N35868	-21	-0.0439	-	7470A	PPB	16 Nov 2019 13:33:31	U	SMPL
K5822-02DUP - 1	N35868DUP	18	-0.0356	-	7470A	PPB	16 Nov 2019 13:35:40	U	SMPL
K5822-02MS - 1	N35868MS	16846	3.5498	-	7470A	PPB	16 Nov 2019 13:37:46	U	SMPL
CCV68 - 1	CCV68	22810	4.8205	-	7470A	PPB	16 Nov 2019 13:44:03	U	SMPL
CCB68 - 1	CCB68	11	-0.0371	-	7470A	PPB	16 Nov 2019 13:46:10	U	SMPL
K5822-02MSD - 1	N35868MSD	16899	3.5611	-	7470A	PPB	16 Nov 2019 13:48:16	U	SMPL
K5665-04LX5 - 1		-13	-0.0422	-	7470A	PPB	16 Nov 2019 13:50:23	U	SMPL
K5807-22LX5 - 1		13	-0.0366	-	7470A	PPB	16 Nov 2019 13:52:30	U	SMPL
K5822-02LX5 - 1		19	-0.0354	-	7470A	PPB	16 Nov 2019 13:54:36	U	SMPL
PB124864TB - 1	PB124815TB	9	-0.0375	-	7470A	PPB	16 Nov 2019 13:56:43	U	SMPL
PB124867TB - 1	PB124829TB	16	-0.0360	-	7470A	PPB	16 Nov 2019 13:58:50	U	SMPL
PB124887TB - 1	PB124790TB	35	-0.0320	-	7470A	PPB	16 Nov 2019 14:00:58	U	SMPL
PB124864BS - 1	LCSW	19206	4.0526	-	7470A	PPB	16 Nov 2019 14:03:06	U	SMPL
CCV69 - 1	CCV69	22271	4.7057	-	7470A	PPB	16 Nov 2019 14:08:03	U	SMPL
CCB69 - 1	CCB69	21	-0.0349	-	7470A	PPB	16 Nov 2019 14:10:09	U	SMPL