


LB106491

INSTRUMENT ID CVI

245.1

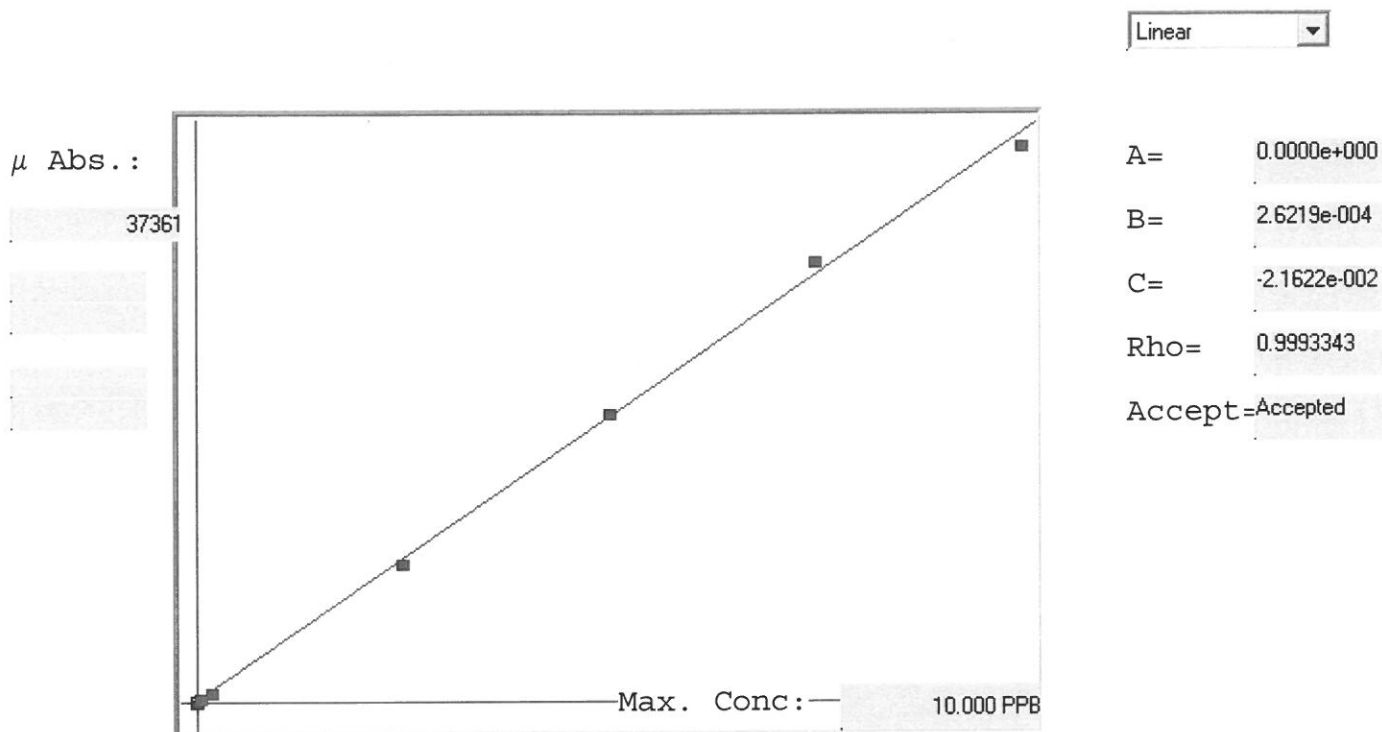

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.016	-0.016	23	0.000	23				
0.05	0.050	0.056	0.006	297	0.0 %	297				
0.2	0.200	0.171	-0.029	733	0.0 %	733				
2.5	2.500	2.427	-0.073	9339	0.0 %	9339				
5.0	5.000	5.086	0.086	19479	0.0 %	19479				
7.5	7.500	7.752	0.252	29649	0.0 %	29649				
10.0	10.000	9.774	-0.226	37361	0.0 %	37361				

LB106491 INSTRUMENT ID CV1

Method: 245.1

Operator: Admin

Date of Analysis: 26 Nov 2019 14:53:43

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	23	-	0.0000	245.1	PPB	26 Nov 2019 14:55:55	S	Std
0.05 - 1	50.05	297	-	0.0500	245.1	PPB	26 Nov 2019 14:58:12	S	Std
0.2 - 1	50.2	733	-	0.2000	245.1	PPB	26 Nov 2019 15:00:30	S	Std
2.5 - 1	52.5	9339	-	2.5000	245.1	PPB	26 Nov 2019 15:04:46	S	Std
5.0 - 1	55.0	19479	-	5.0000	245.1	PPB	26 Nov 2019 15:07:02	S	Std
7.5 - 1	57.5	29649	-	7.5000	245.1	PPB	26 Nov 2019 15:09:18	S	Std
10.0 - 1	510.0	37361	-	10.0000	245.1	PPB	26 Nov 2019 15:14:41	S	Std
ICV09 - 1	ICV09	15017	3.9157	-245.1		PPB	26 Nov 2019 15:17:20	U	SMPL
ICB09 - 1	ICB09	-41	-0.0324	-245.1		PPB	26 Nov 2019 15:19:35	U	SMPL
CCV40 - 1	CCV40	19249	5.0253	-245.1		PPB	26 Nov 2019 15:21:50	U	SMPL
CCB40 - 1	CCB40	-59	-0.0371	-245.1		PPB	26 Nov 2019 15:24:06	U	SMPL
CRA - 1	CRA	270	0.0492	-245.1		PPB	26 Nov 2019 15:26:21	U	SMPL
HighStd - 1	HighStd	36878	9.6475	-245.1		PPB	26 Nov 2019 15:28:37	U	SMPL
ChkStd - 1	ChkStd	26903	7.0321	-245.1		PPB	26 Nov 2019 15:30:52	U	SMPL
PB125137BL - 1	PBW	-93	-0.0460	-245.1		PPB	26 Nov 2019 15:33:08	U	SMPL
PB125137BS - 1	LCSW	14935	3.8942	-245.1		PPB	26 Nov 2019 15:35:24	U	SMPL
K5960-07 - 1	14B-(1-4)-COMP	1085	0.2629	-245.1		PPB	26 Nov 2019 15:37:41	U	SMPL
K5978-10 - 1	14B-(1-4)-COMP	358	0.0722	-245.1		PPB	26 Nov 2019 15:39:57	U	SMPL
K6016-03 - 1	HP-627	-29	-0.0292	-245.1		PPB	26 Nov 2019 15:42:15	U	SMPL
K6031-01 - 1	391114118.1	22	-0.0159	-245.1		PPB	26 Nov 2019 15:44:32	U	SMPL
K6031-01DUP - 1	391114118.1DUP	34	-0.0127	-245.1		PPB	26 Nov 2019 15:46:47	U	SMPL
CCV41 - 1	CCV41	19021	4.9655	-245.1		PPB	26 Nov 2019 15:49:03	U	SMPL
CCB41 - 1	CCB41	-20	-0.0269	-245.1		PPB	26 Nov 2019 15:51:19	U	SMPL
K6031-01MS - 1	391114118.1MS	16846	4.3953	-245.1		PPB	26 Nov 2019 15:53:34	U	SMPL
K6031-01MSD - 1	391114118.1MSD	16983	4.4312	-245.1		PPB	26 Nov 2019 15:55:49	U	SMPL
K6032-01 - 1	391114120.1	-5	-0.0229	-245.1		PPB	26 Nov 2019 15:58:05	U	SMPL
K6033-01 - 1	391114119.1	7	-0.0198	-245.1		PPB	26 Nov 2019 16:00:21	U	SMPL
K6034-01 - 1	391114121.1	14	-0.0180	-245.1		PPB	26 Nov 2019 16:02:37	U	SMPL
K6031-01LX5 - 1		-15	-0.0256	-245.1		PPB	26 Nov 2019 16:04:54	U	SMPL
K6031-01A - 1		16872	4.4021	-245.1		PPB	26 Nov 2019 16:07:10	U	SMPL
CCV42 - 1	CCV42	18883	4.9293	-245.1		PPB	26 Nov 2019 16:09:27	U	SMPL
CCB42 - 1	CCB42	-36	-0.0311	-245.1		PPB	26 Nov 2019 16:11:45	U	SMPL