


28106545
INSTRUMENT ID CVI

245.1

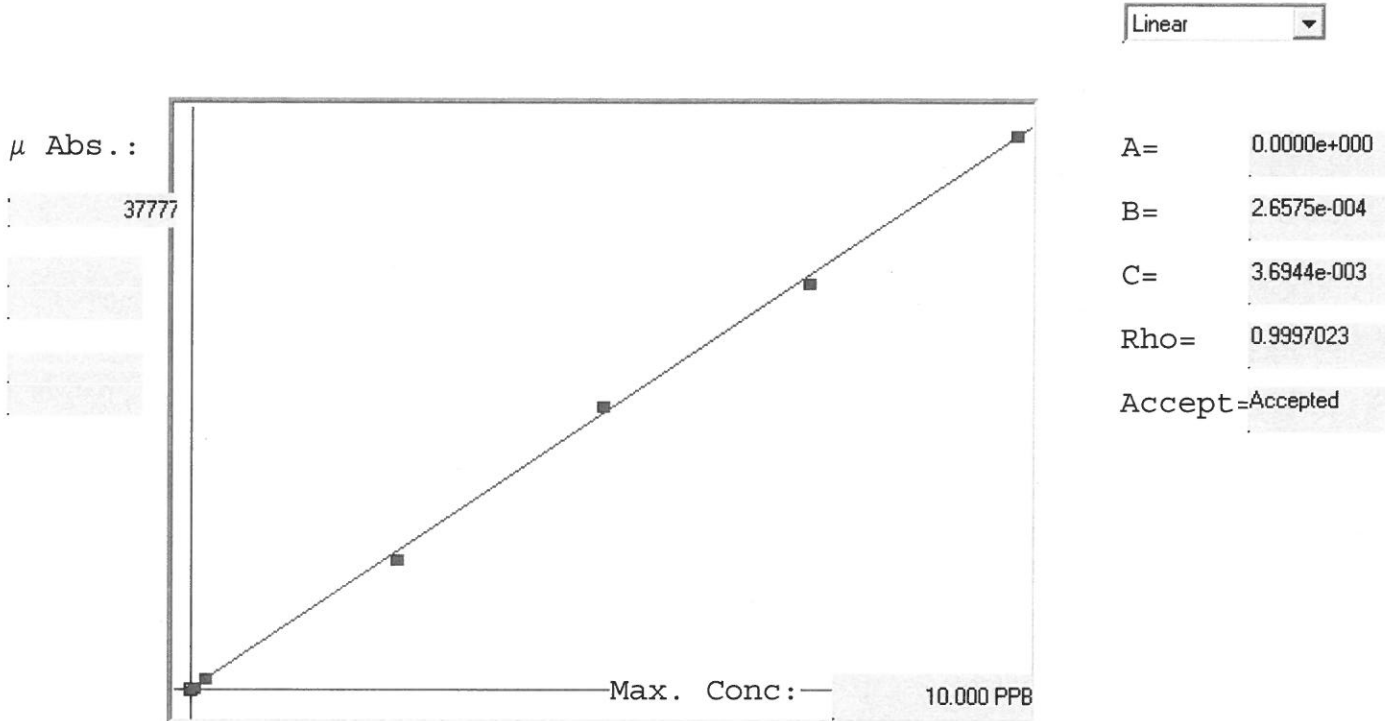

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.006	0.006	7	0.000	7				
0.05	0.050	0.064	0.014	227	0.0 %	227				
0.2	0.200	0.231	0.031	854	0.0 %	854				
2.5	2.500	2.382	-0.118	8949	0.0 %	8949				
5.0	5.000	5.154	0.154	19381	0.0 %	19381				
7.5	7.500	7.371	-0.129	27722	0.0 %	27722				
10.0	10.000	10.043	0.043	37777	0.0 %	37777				

Ib106545 INSTRUMENT ID CV1

Method: 245.1

Operator: Admin

Date of Analysis: 29 Nov 2019 13:01:33

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	7	-	0.0000	245.1	PPB	29 Nov 2019 13:01:50	S	Std
0.05 - 1	50.05	227	-	0.0500	245.1	PPB	29 Nov 2019 13:04:07	S	Std
0.2 - 1	50.2	854	-	0.2000	245.1	PPB	29 Nov 2019 13:06:24	S	Std
2.5 - 1	52.5	8949	-	2.5000	245.1	PPB	29 Nov 2019 13:08:41	S	Std
5.0 - 1	55.0	19381	-	5.0000	245.1	PPB	29 Nov 2019 13:10:58	S	Std
7.5 - 1	57.5	27722	-	7.5000	245.1	PPB	29 Nov 2019 13:13:14	S	Std
10.0 - 1	510.0	37777	-	10.0000	245.1	PPB	29 Nov 2019 13:18:39	S	Std
ICV13 - 1	ICV13	14215	3.7813	-245.1		PPB	29 Nov 2019 13:21:43	U	SMPL
ICB13 - 1	ICB13	0	0.0037	-245.1		PPB	29 Nov 2019 13:23:58	U	SMPL
CCV55 - 1	CCV55	18636	4.9562	-245.1		PPB	29 Nov 2019 13:29:23	U	SMPL
CCB55 - 1	CCB55	-16	-0.0006	-245.1		PPB	29 Nov 2019 13:31:39	U	SMPL
CRA - 1	CRA	228	0.0643	-245.1		PPB	29 Nov 2019 13:39:05	U	SMPL
HighStd - 1	HighStd	35131	9.3397	-245.1		PPB	29 Nov 2019 13:41:20	U	SMPL
ChkStd - 1	ChkStd	24306	6.4630	-245.1		PPB	29 Nov 2019 13:43:36	U	SMPL
PB125180BL - 1	PBW	-55	-0.0109	-245.1		PPB	29 Nov 2019 13:45:52	U	SMPL
PB125180BS - 1	LCSW	14153	3.7648	-245.1		PPB	29 Nov 2019 13:48:09	U	SMPL
K6035-01 - 1	391121719	1	0.0040	-245.1		PPB	29 Nov 2019 13:50:25	U	SMPL
K6035-01DUP - 1	391121719DUP	45	0.0157	-245.1		PPB	29 Nov 2019 13:52:42	U	SMPL
K6035-01MS - 1	391121719MS	17563	4.6711	-245.1		PPB	29 Nov 2019 13:54:59	U	SMPL
K6035-01MSD - 1	391121719MSD	17102	4.5485	-245.1		PPB	29 Nov 2019 13:57:48	U	SMPL
K6036-01 - 1	391121720	344	0.0951	-245.1		PPB	29 Nov 2019 14:00:05	U	SMPL
CCV56 - 1	CCV56	18520	4.9254	-245.1		PPB	29 Nov 2019 14:02:21	U	SMPL
CCB56 - 1	CCB56	-47	-0.0088	-245.1		PPB	29 Nov 2019 14:04:36	U	SMPL
K6042-01 - 1	391120026.0	380	0.1047	-245.1		PPB	29 Nov 2019 14:06:52	U	SMPL
K6043-01 - 1	391120746.0	380	0.1047	-245.1		PPB	29 Nov 2019 14:09:07	U	SMPL
K6044-01 - 1	391120753.0	-54	-0.0107	-245.1		PPB	29 Nov 2019 14:11:23	U	SMPL
K6045-01 - 1	391120772.0-33466	88	0.0271	-245.1		PPB	29 Nov 2019 14:13:37	U	SMPL
K6046-01 - 1	391119066.0	13	0.0071	-245.1		PPB	29 Nov 2019 14:15:53	U	SMPL
K6047-01 - 1	391121077.0	18988	5.0497	-245.1		PPB	29 Nov 2019 14:18:07	U	SMPL
K6048-01 - 1	391120731.1-SM19-1059	-95	-0.0216	-245.1		PPB	29 Nov 2019 14:20:24	U	SMPL
K6049-01 - 1	39120729.1-WW19-1549	-14	-0.0000	-245.1		PPB	29 Nov 2019 14:22:43	U	SMPL
K6050-01 - 1	391120732.1-OC19-586	15	0.0077	-245.1		PPB	29 Nov 2019 14:25:01	U	SMPL
K6051-01 - 1	391120727.1-WW19-1549	69	0.0220	-245.1		PPB	29 Nov 2019 14:27:16	U	SMPL
CCV57 - 1	CCV57	18576	4.9403	-245.1		PPB	29 Nov 2019 14:29:32	U	SMPL
CCB57 - 1	CCB57	-25	-0.0029	-245.1		PPB	29 Nov 2019 14:31:47	U	SMPL
K6072-01 - 1	391107002	98	0.0297	-245.1		PPB	29 Nov 2019 14:34:03	U	SMPL
K6035-01LX5 - 1		-29	-0.0040	-245.1		PPB	29 Nov 2019 14:36:18	U	SMPL
K6035-01A - 1		14415	3.8345	-245.1		PPB	29 Nov 2019 14:38:34	U	SMPL
CCV58 - 1	CCV58	18947	5.0388	-245.1		PPB	29 Nov 2019 14:40:49	U	SMPL
CCB58 - 1	CCB58	-75	-0.0162	-245.1		PPB	29 Nov 2019 14:43:06	U	SMPL