


LB106605
INSTRUMENT ID CV1

7470A

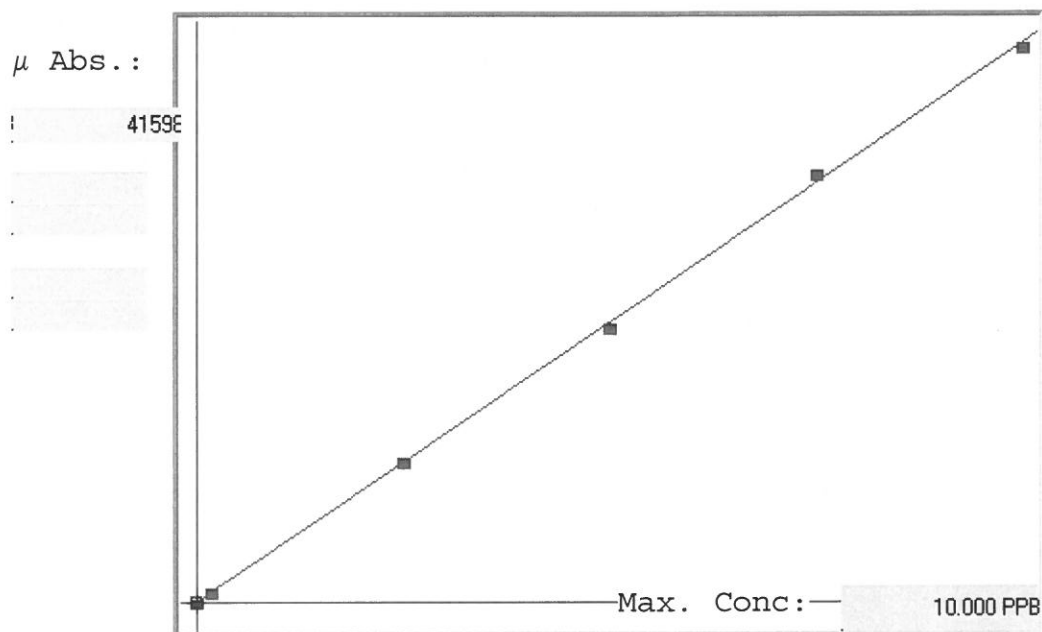

Linear

A= 0.0000e+000

B= 2.3819e-004

C= 1.0818e-003

Rho= 0.9997212

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.014	0.014	55	0.000	55				
0.2	0.200	0.185	-0.015	771	0.0 %	771				
2.5	2.500	2.509	0.009	10528	0.0 %	10528				
5.0	5.000	4.912	-0.088	20618	0.0 %	20618				
7.5	7.500	7.671	0.171	32199	0.0 %	32199				
10.0	10.000	9.909	-0.091	41598	0.0 %	41598				

LB106605 INSTRUMENT ID CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 Dec 2019 13:13:17

Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc.	Method	Units	Date	Type	Type
0.0 - 1	50.0	55	-	0.0000	7470A	PPB	05 Dec 2019 13:13:32	S	Std
0.2 - 1	50.2	771	-	0.2000	7470A	PPB	05 Dec 2019 13:15:40	S	Std
2.5 - 1	52.5	10528	-	2.5000	7470A	PPB	05 Dec 2019 13:17:48	S	Std
5.0 - 1	55.0	20618	-	5.0000	7470A	PPB	05 Dec 2019 13:19:55	S	Std
7.5 - 1	57.5	32199	-	7.5000	7470A	PPB	05 Dec 2019 13:22:03	S	Std
10.0 - 1	510.0	41598	-	10.0000	7470A	PPB	05 Dec 2019 13:24:10	S	Std
ICV18 - 1	ICV18	15989	3.8096	-	7470A	PPB	05 Dec 2019 13:26:40	U	SMPL
ICB18 - 1	ICB18	-14	-0.0023	-	7470A	PPB	05 Dec 2019 13:28:46	U	SMPL
CCV73 - 1	CCV73	20618	4.9122	-	7470A	PPB	05 Dec 2019 13:30:52	U	SMPL
CCB73 - 1	CCB73	2	0.0016	-	7470A	PPB	05 Dec 2019 13:32:59	U	SMPL
CRA - 1	CRA	769	0.1843	-	7470A	PPB	05 Dec 2019 13:35:06	U	SMPL
HighStd - 1	HighStd	41466	9.8780	-	7470A	PPB	05 Dec 2019 13:37:13	U	SMPL
ChkStd - 1	ChkStd	30006	7.1483	-	7470A	PPB	05 Dec 2019 13:39:19	U	SMPL
PB125261BL - 1	PBW	49	0.0128	-	7470A	PPB	05 Dec 2019 13:41:26	U	SMPL
PB125261BS - 1	LCSW	16162	3.8508	-	7470A	PPB	05 Dec 2019 13:43:33	U	SMPL
K6112-04 - 1	OK-02-120419	46	0.0120	-	7470A	PPB	05 Dec 2019 13:45:40	U	SMPL
K6112-04DUP - 1	OK-02-120419DUP	66	0.0168	-	7470A	PPB	05 Dec 2019 13:47:48	U	SMPL
K6112-04MS - 1	OK-02-120419MS	16576	3.9494	-	7470A	PPB	05 Dec 2019 13:49:55	U	SMPL
K6112-04MSD - 1	OK-02-120419MSD	16654	3.9680	-	7470A	PPB	05 Dec 2019 13:52:03	U	SMPL
K6135-07 - 1	COMP-34	11	0.0037	-	7470A	PPB	05 Dec 2019 13:54:10	U	SMPL
CCV74 - 1	CCV74	20633	4.9157	-	7470A	PPB	05 Dec 2019 13:56:16	U	SMPL
CCB74 - 1	CCB74	38	0.0101	-	7470A	PPB	05 Dec 2019 13:58:23	U	SMPL
K6135-08 - 1	COMP-35	39	0.0104	-	7470A	PPB	05 Dec 2019 14:00:29	U	SMPL
K6135-09 - 1	COMP-36	45	0.0118	-	7470A	PPB	05 Dec 2019 14:02:35	U	SMPL
K6141-05 - 1	CMJ-01-COMP	58	0.0149	-	7470A	PPB	05 Dec 2019 14:04:41	U	SMPL
K6112-04LX5 - 1		36	0.0097	-	7470A	PPB	05 Dec 2019 14:06:48	U	SMPL
PB125261TB - 1	PB125248TB	59	0.0151	-	7470A	PPB	05 Dec 2019 14:08:55	U	SMPL
CCV75 - 1	CCV75	20548	4.8955	-	7470A	PPB	05 Dec 2019 14:11:02	U	SMPL
CCB75 - 1	CCB75	38	0.0101	-	7470A	PPB	05 Dec 2019 14:13:09	U	SMPL