

106634

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AL

Instrument ID : Konelab

12/6/2019 11:39

Test: ~~Total~~ ^{Reactive} CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.303	0.0	0.111	
ICB1	0.074	0.0	0.002	
CCV1	243.848	0.0	0.277	
CCB1	-0.011	0.0	0.002	
PB125272BL	-0.080	0.0	0.002	
K6113-05	-0.109	0.0	0.002	
K6113-05DUP	-0.331	0.0	0.002	
K6141-05	-0.371	0.0	0.002	
K6145-02	-0.211	0.0	0.002	
K6145-04	-0.292	0.0	0.002	
K6145-06	-0.208	0.0	0.002	
K6162-03	-0.525	0.0	0.002	
K6164-03	-0.104	0.0	0.002	
PB125290BL	-0.043	0.0	0.002	
CCV2	246.296	0.0	0.280	
CCB2	0.025	0.0	0.002	
K6174-05	-0.074	0.0	0.002	
K6174-05DUP	-0.308	0.0	0.002	
CCV3	250.508	0.0	0.284	
CCB3	-0.025	0.0	0.002	

N	20
Mean	41.718
SD	91.0018
CV%	218.13

Aquakem v. 7.2AQ1

AE

Results from time period:

Fri Dec 06 11:25:09 2019

Fri Dec 06 11:31:56 2019

Sample Id	Sam/Ctr/c/	Test short Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive Cl P	-0.6774	µg/l	12/6/2019 10:11:10	
5.OPPBCN	A	Reactive Cl P	4.1606	µg/l	12/6/2019 10:11:11	
10PPBCN	A	Reactive Cl P	9.1626	µg/l	12/6/2019 10:11:12	
50PPBCN	A	Reactive Cl P	49.4944	µg/l	12/6/2019 10:11:13	
100PPBCN	A	Reactive Cl P	101.8458	µg/l	12/6/2019 10:11:14	
250PPBCN	A	Reactive Cl P	252.6148	µg/l	12/6/2019 10:11:15	
500PPBCN	A	Reactive Cl P	498.3992	µg/l	12/6/2019 10:11:16	
ICV1	S	Reactive Cl P	96.3031	µg/l	12/6/2019 11:25:09	
ICB1	S	Reactive Cl P	0.0737	µg/l	12/6/2019 11:25:10	
CCV1	S	Reactive Cl P	243.8482	µg/l	12/6/2019 11:25:11	
CCB1	S	Reactive Cl P	-0.0111	µg/l	12/6/2019 11:25:12	
PB125272BL	S	Reactive Cl P	-0.0797	µg/l	12/6/2019 11:25:13	
K6113-05	S	Reactive Cl P	-0.1091	µg/l	12/6/2019 11:25:14	
K6113-05DUP	S	Reactive Cl P	-0.3308	µg/l	12/6/2019 11:25:15	
K6141-05	S	Reactive Cl P	-0.371	µg/l	12/6/2019 11:25:16	
K6145-02	S	Reactive Cl P	-0.2114	µg/l	12/6/2019 11:25:17	
K6145-04	S	Reactive Cl P	-0.2924	µg/l	12/6/2019 11:25:18	
K6145-06	S	Reactive Cl P	-0.2083	µg/l	12/6/2019 11:25:19	
K6162-03	S	Reactive Cl P	-0.5249	µg/l	12/6/2019 11:31:48	
K6164-03	S	Reactive Cl P	-0.104	µg/l	12/6/2019 11:31:49	
PB125290BL	S	Reactive Cl P	-0.0431	µg/l	12/6/2019 11:31:50	
CCV2	S	Reactive Cl P	246.2964	µg/l	12/6/2019 11:31:51	
CCB2	S	Reactive Cl P	0.025	µg/l	12/6/2019 11:31:52	
K6174-05	S	Reactive Cl P	-0.0738	µg/l	12/6/2019 11:31:53	
K6174-05DUP	S	Reactive Cl P	-0.3077	µg/l	12/6/2019 11:31:54	
CCV3	S	Reactive Cl P	250.5078	µg/l	12/6/2019 11:31:55	
CCB3	S	Reactive Cl P	-0.0248	µg/l	12/6/2019 11:31:56	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

12/6/2019 10:12


Test Total CN

Accepted 12/6/2019 10:12

Factor 888.3
Bias 0.002

Coeff. of det. 0.999927

Errors

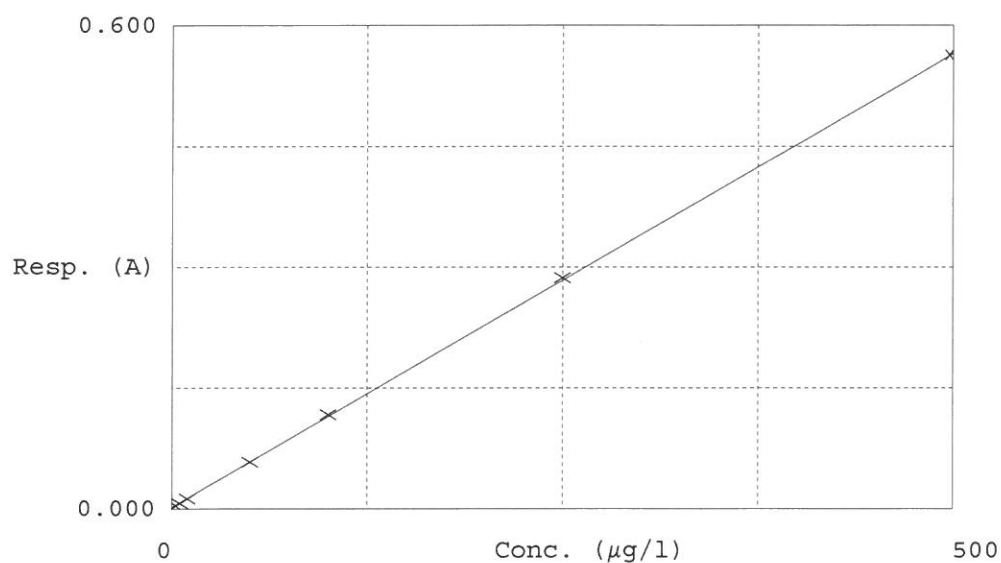

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.6774	0.0000	
2	5.0PPBCN	0.007	4.1606	5.0000	
3	10PPBCN	0.013	9.1626	10.0000	
4	50PPBCN	0.058	49.4944	50.0000	
5	100PPBCN	0.117	101.8458	100.0000	
6	250PPBCN	0.287	252.6148	250.0000	
7	500PPBCN	0.563	498.3992	500.0000	