

15106661

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : DK

Instrument ID : Konelab

12/9/2019 15:48

Test: Total CN

mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.985	0.0	0.109	
ICB1	0.984	0.0	0.002	
CCV1	237.436	0.0	0.265	
CCB1	1.089	0.0	0.002	
PB125318BL	0.563	0.0	0.002	
K6111-08	0.518	0.0	0.002	
K6111-08DUP	0.540	0.0	0.002	
K6117-03	0.353	0.0	0.002	
K6118-05	0.557	0.0	0.002	
K6186-01	0.621	0.0	0.002	
K6188-03	0.607	0.0	0.002	
K6188-07	0.615	0.0	0.002	
CCV2	253.033	0.0	0.283	
CCB2	0.630	0.0	0.002	

N	14
Mean	42.467
SD	89.6854
CV%	211.19

LB106661

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : De

Instrument ID : Konelab

12/9/2019 13:52

Test Total CN


Accepted 12/9/2019 13:52

Factor 898.9

Bias 0.001

Coeff. of det. 0.999861

Errors

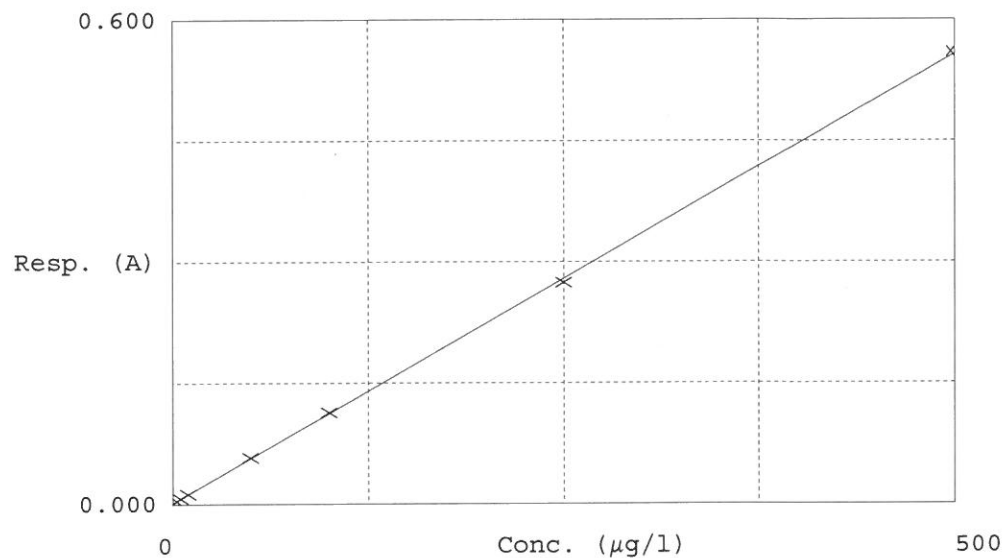

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.4227	0.0000	
2	5.0PPBCN	0.007	5.3340	5.0000	
3	10PPBCN	0.012	10.0966	10.0000	
4	50PPBCN	0.058	50.7344	50.0000	
5	100PPBCN	0.114	101.0637	100.0000	
6	250PPBCN	0.274	245.2802	250.0000	
7	500PPBCN	0.560	502.0684	500.0000	

LB106661

Aquakem v. 7.2AQ1

Results from time period:

Mon Dec 09 15:41:08 2019

Mon Dec 09 15:45:01 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	Cl P	0.4227	µg/l	12/9/2019 13:42:56	
5.OPPBCN	A	Reactive	Cl P	5.334	µg/l	12/9/2019 13:42:57	
10PPBCN	A	Reactive	Cl P	10.0966	µg/l	12/9/2019 13:42:58	
50PPBCN	A	Reactive	Cl P	50.7344	µg/l	12/9/2019 13:42:59	
100PPBCN	A	Reactive	Cl P	101.0637	µg/l	12/9/2019 13:43:00	
250PPBCN	A	Reactive	Cl P	245.2802	µg/l	12/9/2019 13:43:01	
500PPBCN	A	Reactive	Cl P	502.0684	µg/l	12/9/2019 13:43:02	
ICV1	S	Reactive	Cl P	96.9847	µg/l	12/9/2019 15:41:08	
ICB1	S	Reactive	Cl P	0.9845	µg/l	12/9/2019 15:41:09	
CCV1	S	Reactive	Cl P	237.4364	µg/l	12/9/2019 15:41:10	
CCB1	S	Reactive	Cl P	1.0892	µg/l	12/9/2019 15:41:11	
PB125318BL	S	Reactive	Cl P	0.5633	µg/l	12/9/2019 15:41:12	
K6111-08	S	Reactive	Cl P	0.5183	µg/l	12/9/2019 15:41:13	
K6111-08DUP	S	Reactive	Cl P	0.5404	µg/l	12/9/2019 15:41:14	
K6117-03	S	Reactive	Cl P	0.3532	µg/l	12/9/2019 15:41:15	
K6118-05	S	Reactive	Cl P	0.5569	µg/l	12/9/2019 15:41:16	
K6186-01	S	Reactive	Cl P	0.6209	µg/l	12/9/2019 15:41:17	
K6188-03	S	Reactive	Cl P	0.6075	µg/l	12/9/2019 15:41:18	
K6188-07	S	Reactive	Cl P	0.6145	µg/l	12/9/2019 15:44:59	
CCV2	S	Reactive	Cl P	253.0333	µg/l	12/9/2019 15:45:00	
CCB2	S	Reactive	Cl P	0.6296	µg/l	12/9/2019 15:45:01	