


LB106662
INSTRUMENT ID: CWI

7470A

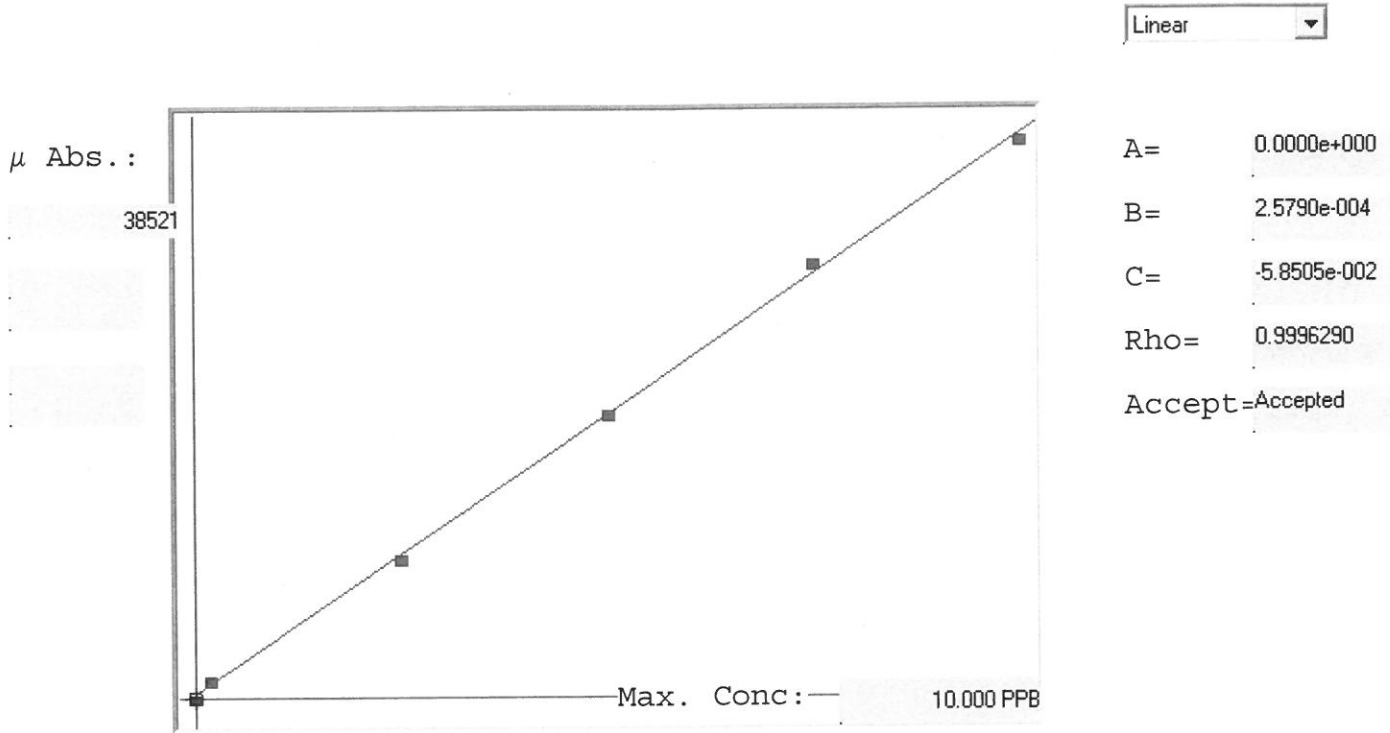

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.048	-0.048	40	0.000	40				
0.2	0.200	0.266	0.066	1260	0.0 %	1260				
2.5	2.500	2.427	-0.073	9637	0.0 %	9637				
5.0	5.000	4.997	-0.003	19603	0.0 %	19603				
7.5	7.500	7.682	0.182	30014	0.0 %	30014				
10.0	10.000	9.876	-0.124	38521	0.0 %	38521				

LB106668 INSTRUMENT ID CV1

Method: 7470A

Operator: Admin

Date of Analysis: 10 Dec 2019 10:49:43

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	30.0	40	-	0.00007470A	PPB	10 Dec 2019 10:53:22	S	Std
0.2 - 1	50.2	1260	-	0.20007470A	PPB	10 Dec 2019 10:56:58	S	Std
2.5 - 1	52.5	9637	-	2.50007470A	PPB	10 Dec 2019 10:59:06	S	Std
5.0 - 1	65.0	19603	-	5.00007470A	PPB	10 Dec 2019 11:01:13	S	Std
7.5 - 1	57.5	30014	-	7.50007470A	PPB	10 Dec 2019 11:03:21	S	Std
10.0 - 1	510.0	38521	-	10.00007470A	PPB	10 Dec 2019 11:14:01	S	Std
ICV21 - 1	ICV21	16128	4.1008	-7470A	PPB	10 Dec 2019 11:16:29	U	SMPL
ICB21 - 1	ICB21	-25	-0.0650	-7470A	PPB	10 Dec 2019 11:18:35	U	SMPL
CCV85 - 1	CCV85	19047	4.8536	-7470A	PPB	10 Dec 2019 11:20:41	U	SMPL
CCB85 - 1	CCB85	-19	-0.0634	-7470A	PPB	10 Dec 2019 11:22:47	U	SMPL
CRA - 1	CRA	1224	0.2572	-7470A	PPB	10 Dec 2019 11:24:54	U	SMPL
HighStd - 1	HighStd	37863	9.7062	-7470A	PPB	10 Dec 2019 11:27:00	U	SMPL
ChkStd - 1	ChkStd	28298	7.2394	-7470A	PPB	10 Dec 2019 11:29:07	U	SMPL
PB125323BL - 1	PBW	-59	-0.0737	-7470A	PPB	10 Dec 2019 11:31:13	U	SMPL
PB125323BS - 1	LCSW	15975	4.0614	-7470A	PPB	10 Dec 2019 11:34:57	U	SMPL
K6134-01 - 1	30573	222	-0.0013	-7470A	PPB	10 Dec 2019 11:37:04	U	SMPL
K6134-01DUP - 1	30573DUP	95	-0.0340	-7470A	PPB	10 Dec 2019 11:39:11	U	SMPL
K6134-01MS - 1	30573MS	13996	3.5510	-7470A	PPB	10 Dec 2019 11:41:19	U	SMPL
K6134-01MSD - 1	30573MSD	14492	3.6789	-7470A	PPB	10 Dec 2019 11:43:27	U	SMPL
K6174-04 - 1	WATER-COMP	-24	-0.0647	-7470A	PPB	10 Dec 2019 11:45:34	U	SMPL
CCV86 - 1	CCV86	19577	4.9903	-7470A	PPB	10 Dec 2019 11:47:40	U	SMPL
CCB86 - 1	CCB86	2	-0.0580	-7470A	PPB	10 Dec 2019 11:49:46	U	SMPL
K6196-01 - 1	TW-4	65	-0.0417	-7470A	PPB	10 Dec 2019 11:51:53	U	SMPL
K6196-02 - 1	TW-1	48	-0.0461	-7470A	PPB	10 Dec 2019 11:53:59	U	SMPL
K6196-04 - 1	TW-3	365	0.0356	-7470A	PPB	10 Dec 2019 11:56:05	U	SMPL
K6197-02 - 1	WC-GW	18	-0.0539	-7470A	PPB	10 Dec 2019 11:58:12	U	SMPL
PB125324BL - 1	PBW	2	-0.0580	-7470A	PPB	10 Dec 2019 12:00:19	U	SMPL
PB125324BS - 1	LCSW	16012	4.0709	-7470A	PPB	10 Dec 2019 12:02:26	U	SMPL
K6196-06 - 1	TW-4	13	-0.0552	-7470A	PPB	10 Dec 2019 12:04:34	U	SMPL
K6196-06DUP - 1	TW-4DUP	28	-0.0513	-7470A	PPB	10 Dec 2019 12:06:42	U	SMPL
K6196-06MS - 1	TW-4MS	16497	4.1960	-7470A	PPB	10 Dec 2019 12:08:50	U	SMPL
K6196-06MSD - 1	TW-4MSD	16625	4.2290	-7470A	PPB	10 Dec 2019 12:10:57	U	SMPL
CCV87 - 1	CCV87	20047	5.1115	-7470A	PPB	10 Dec 2019 12:13:03	U	SMPL
CCB87 - 1	CCB87	-20	-0.0637	-7470A	PPB	10 Dec 2019 12:15:09	U	SMPL
K6196-07 - 1	TW-1	40	-0.0482	-7470A	PPB	10 Dec 2019 12:17:15	U	SMPL
K6196-08 - 1	TW-3	42	-0.0477	-7470A	PPB	10 Dec 2019 12:19:21	U	SMPL
PB125325BL - 1	PBW	-6	-0.0601	-7470A	PPB	10 Dec 2019 12:21:27	U	SMPL
PB125325BS - 1	LCSW	15642	3.9755	-7470A	PPB	10 Dec 2019 12:23:32	U	SMPL
K6113-05 - 1	OR-03-120519	16	-0.0544	-7470A	PPB	10 Dec 2019 12:25:39	U	SMPL
K6113-05DUP - 1	OR-03-120519DUP	35	-0.0495	-7470A	PPB	10 Dec 2019 12:27:46	U	SMPL
K6113-05MS - 1	OR-03-120519MS	14883	3.7798	-7470A	PPB	10 Dec 2019 12:29:54	U	SMPL
K6113-05MSD - 1	OR-03-120519MSD	15143	3.8468	-7470A	PPB	10 Dec 2019 12:32:01	U	SMPL
K6147-12 - 1	P001-WC001	20	-0.0533	-7470A	PPB	10 Dec 2019 12:34:10	U	SMPL
K6147-13 - 1	P001-WC002	47	-0.0464	-7470A	PPB	10 Dec 2019 12:36:16	U	SMPL
CCV88 - 1	CCV88	18883	4.8113	-7470A	PPB	10 Dec 2019 12:38:23	U	SMPL
CCB88 - 1	CCB88	16	-0.0544	-7470A	PPB	10 Dec 2019 12:40:30	U	SMPL
K6147-14 - 1	P001-WC003	42	-0.0477	-7470A	PPB	10 Dec 2019 12:42:37	U	SMPL
K6147-15 - 1	P001-WC004	72	-0.0399	-7470A	PPB	10 Dec 2019 12:44:43	U	SMPL
K6147-16 - 1	P001-WC005	39	-0.0484	-7470A	PPB	10 Dec 2019 12:46:50	U	SMPL
K6147-17 - 1	P001-WC006	44	-0.0472	-7470A	PPB	10 Dec 2019 12:48:57	U	SMPL
K6147-18 - 1	P001-WC007	65	-0.0417	-7470A	PPB	10 Dec 2019 12:51:04	U	SMPL
K6147-19 - 1	P001-WC008	76	-0.0389	-7470A	PPB	10 Dec 2019 12:53:11	U	SMPL
K6147-20 - 1	P001-WC009	47	-0.0464	-7470A	PPB	10 Dec 2019 12:55:19	U	SMPL
K6147-21 - 1	P001-WC010	43	-0.0474	-7470A	PPB	10 Dec 2019 12:57:27	U	SMPL
K6147-22 - 1	P001-WC011	119	-0.0278	-7470A	PPB	10 Dec 2019 12:59:35	U	SMPL
K6162-03 - 1	WC	147	-0.0206	-7470A	PPB	10 Dec 2019 13:01:42	U	SMPL
CCV89 - 1	CCV89	19259	4.9083	-7470A	PPB	10 Dec 2019 13:03:48	U	SMPL
CCB89 - 1	CCB89	10	-0.0559	-7470A	PPB	10 Dec 2019 13:05:55	U	SMPL
K6164-03 - 1	BOX-2512	69	-0.0407	-7470A	PPB	10 Dec 2019 13:08:02	U	SMPL
K6174-03 - 1	SOLID-COMP	105	-0.0314	-7470A	PPB	10 Dec 2019 13:10:09	U	SMPL
PB125326BL - 1	PBW	100	-0.0327	-7470A	PPB	10 Dec 2019 13:12:16	U	SMPL
PB125326BS - 1	LCSW	16030	4.0756	-7470A	PPB	10 Dec 2019 13:14:22	U	SMPL
K6111-08 - 1	CL-01-120619	47	-0.0464	-7470A	PPB	10 Dec 2019 13:16:29	U	SMPL
K6111-08DUP - 1	CL-01-120619DUP	2	-0.0580	-7470A	PPB	10 Dec 2019 13:18:36	U	SMPL
K6111-08MS - 1	CL-01-120619MS	14796	3.7573	-7470A	PPB	10 Dec 2019 13:20:41	U	SMPL
K6111-08MSD - 1	CL-01-120619MSD	15129	3.8432	-7470A	PPB	10 Dec 2019 13:22:49	U	SMPL
K6117-03 - 1	TR-04-120619	104	-0.0317	-7470A	PPB	10 Dec 2019 13:24:57	U	SMPL
K6118-05 - 1	SU-02-120619	112	-0.0296	-7470A	PPB	10 Dec 2019 13:27:04	U	SMPL
CCV90 - 1	CCV90	19362	4.9349	-7470A	PPB	10 Dec 2019 13:29:11	U	SMPL
CCB90 - 1	CCB90	10	-0.0559	-7470A	PPB	10 Dec 2019 13:31:18	U	SMPL
K6176-05 - 1	42-SPRUCE	109	-0.0304	-7470A	PPB	10 Dec 2019 13:33:25	U	SMPL
K6176-06 - 1	48-SPRUCE	63	-0.0423	-7470A	PPB	10 Dec 2019 13:35:32	U	SMPL
K6186-01 - 1	S32-GAC-IDW01	9	-0.0562	-7470A	PPB	10 Dec 2019 13:37:39	U	SMPL
K6188-03 - 1	SOIL-COMP-1	47	-0.0464	-7470A	PPB	10 Dec 2019 13:39:44	U	SMPL
K6188-07 - 1	SOIL-COMP-2	36	-0.0492	-7470A	PPB	10 Dec 2019 13:41:51	U	SMPL
K6194-03 - 1	WC-01	58	-0.0435	-7470A	PPB	10 Dec 2019 13:43:59	U	SMPL
PB125327BL - 1	PBW	41	-0.0479	-7470A	PPB	10 Dec 2019 13:46:06	U	SMPL
PB125327BS - 1	LCSW	15780	4.0111	-7470A	PPB	10 Dec 2019 13:48:14	U	SMPL
K6174-05 - 1	WATER-COMP	15	-0.0546	-7470A	PPB	10 Dec 2019 13:50:22	U	SMPL
K6174-05DUP - 1	WATER-COMPDUP	51	-0.0454	-7470A	PPB	10 Dec 2019 13:52:29	U	SMPL
CCV91 - 1	CCV91	19805	5.0491	-7470A	PPB	10 Dec 2019 13:54:36	U	SMPL

LB106668 INSTRUMENT ID CV1

Method: 7470A

Operator: Admin

Date of Analysis: 10 Dec 2019 10:49:43

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
CCB91 - 1	CCB91	2	-0.0580		-7470A	PPB	10 Dec 2019 13:56:43	U	SMPL
K6174-05MS - 1	WATER-COMPMS	15733	3.9990		-7470A	PPB	10 Dec 2019 13:58:50	U	SMPL
K6174-05MSD - 1	WATER-COMPMSD	15692	3.9884		-7470A	PPB	10 Dec 2019 14:00:58	U	SMPL
K6179-01 - 1	UC-11-26-19	1952	0.4449		-7470A	PPB	10 Dec 2019 14:03:05	U	SMPL
K6134-01LX5 - 1		-646	-0.2251		-7470A	PPB	10 Dec 2019 14:05:12	U	SMPL
K6196-06LX5 - 1		-318	-0.1405		-7470A	PPB	10 Dec 2019 14:07:23	U	SMPL
K6113-05LX5 - 1		-205	-0.1114		-7470A	PPB	10 Dec 2019 14:09:31	U	SMPL
K6111-08LX5 - 1		-115	-0.0882		-7470A	PPB	10 Dec 2019 14:11:39	U	SMPL
K6174-05LX5 - 1		-145	-0.0959		-7470A	PPB	10 Dec 2019 14:13:46	U	SMPL
PB125325TB - 1	PB125257TB	-58	-0.0735		-7470A	PPB	10 Dec 2019 14:15:54	U	SMPL
PB125326TB - 1	PB125297TB	-45	-0.0701		-7470A	PPB	10 Dec 2019 14:18:01	U	SMPL
CCV92 - 1	CCV92	20229	5.1585		-7470A	PPB	10 Dec 2019 14:20:09	U	SMPL
CCB92 - 1	CCB92	-34	-0.0673		-7470A	PPB	10 Dec 2019 14:22:15	U	SMPL
PB125327TB - 1	PB125299TB	37	-0.0490		-7470A	PPB	10 Dec 2019 14:24:23	U	SMPL
CCV93 - 1	CCV93	19847	5.0600		-7470A	PPB	10 Dec 2019 14:26:30	U	SMPL
CCB93 - 1	CCB93	-10	-0.0611		-7470A	PPB	10 Dec 2019 14:28:36	U	SMPL