


LB106711
INSTRUMENT ID 001

7470A

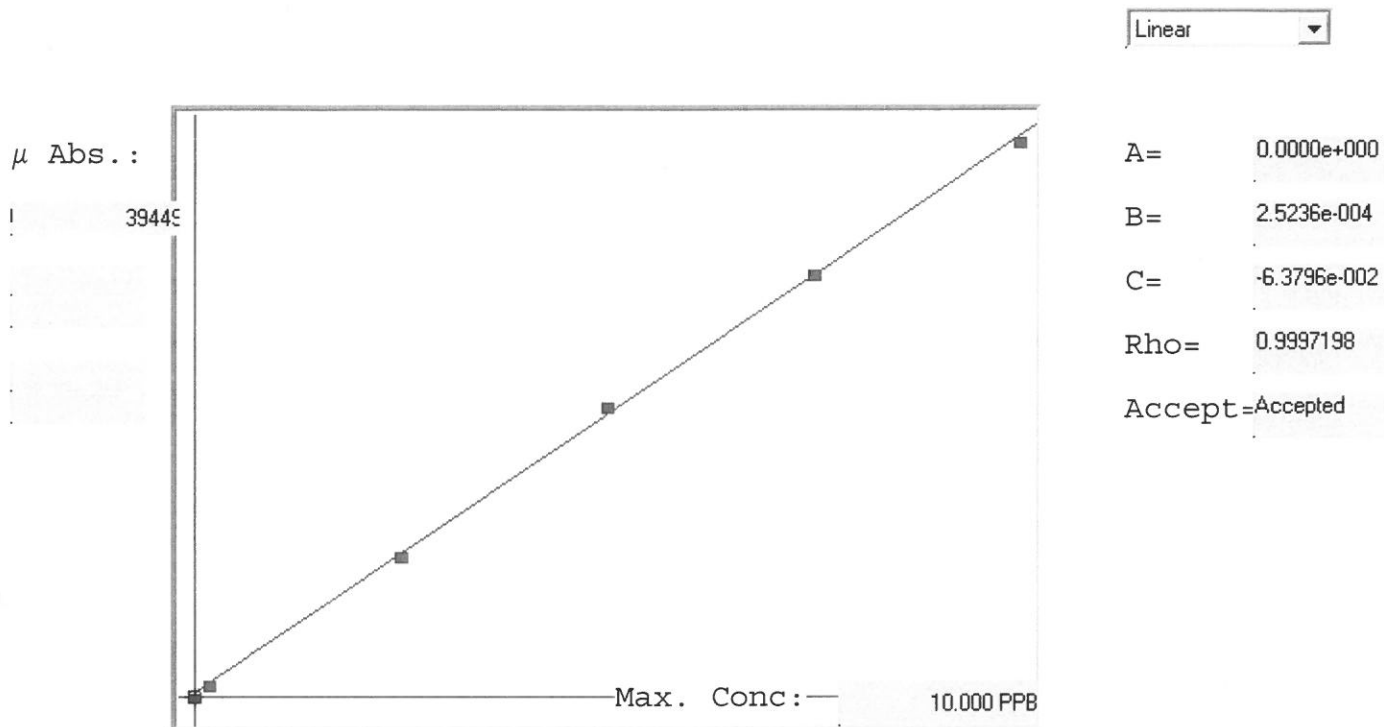

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.032	-0.032	127	0.000	127				
0.2	0.200	0.160	-0.040	888	0.0 %	888				
2.5	2.500	2.474	-0.026	10058	0.0 %	10058				
5.0	5.000	5.172	0.172	20748	0.0 %	20748				
7.5	7.500	7.534	0.034	30106	0.0 %	30106				
10.0	10.000	9.891	-0.109	39449	0.0 %	39449				

LB106711 INSTRUMENT ID CV1

Method: 7470A

Operator: Admin

Date of Analysis: 12 Dec 2019 10:31:25

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1		127	-	0.0000	7470A	PPB	12 Dec 2019 10:40:53	S	Std
0.2 - 1		888	-	0.2000	7470A	PPB	12 Dec 2019 10:43:01	S	Std
2.5 - 1		10058	-	2.5000	7470A	PPB	12 Dec 2019 10:45:09	S	Std
5.0 - 1		20748	-	5.0000	7470A	PPB	12 Dec 2019 10:47:17	S	Std
7.5 - 1		30106	-	7.5000	7470A	PPB	12 Dec 2019 10:49:25	S	Std
10.0 - 1		39449	-	10.0000	7470A	PPB	12 Dec 2019 10:51:31	S	Std
ICV26 - 1	ICV26	15812	3.9264 ✓		7470A	PPB	12 Dec 2019 10:54:27	U	SMPL
ICB26 - 1	ICB26	247	-0.0015 ✓		7470A	PPB	12 Dec 2019 10:56:33	U	SMPL
CCV09 - 1	CCV09	20799	5.1849 ✓		7470A	PPB	12 Dec 2019 10:58:40	U	SMPL
CCB09 - 1	CCB09	242	-0.0027 ✓		7470A	PPB	12 Dec 2019 11:00:46	U	SMPL
CRA - 1	CRA	884	0.1593 ✓		7470A	PPB	12 Dec 2019 11:02:52	U	SMPL
HighStd - 1	HighStd	39566	9.9209 ✓		7470A	PPB	12 Dec 2019 11:04:58	U	SMPL
ChkStd - 1	ChkStd	27489	6.8732 ✓		7470A	PPB	12 Dec 2019 11:07:04	U	SMPL
PB125400BL - 1	PBW	-22	-0.0693 ✓		7470A	PPB	12 Dec 2019 11:09:11	U	SMPL
PB125400BS - 1	LCSW	15907	3.9504 ✓		7470A	PPB	12 Dec 2019 11:11:18	U	SMPL
K6204-14 - 1	K072-AA-WC-1	16	-0.0598 ✓		7470A	PPB	12 Dec 2019 11:13:25	U	SMPL
K6204-14DUP - 1	K072-AA-WC-1DUP	38	-0.0542 ✓		7470A	PPB	12 Dec 2019 11:15:32	U	SMPL
K6204-14MS - 1	K072-AA-WC-1MS	17282	4.2974 ✓		7470A	PPB	12 Dec 2019 11:17:40	U	SMPL
K6204-14MSD - 1	K072-AA-WC-1MSD	17306	4.3035 ✓		7470A	PPB	12 Dec 2019 11:19:48	U	SMPL
K6204-15 - 1	K072-AA-WC-2	491	0.0601 ✓		7470A	PPB	12 Dec 2019 11:21:54	U	SMPL
CCV10 - 1	CCV10	20460	5.0994 ✓		7470A	PPB	12 Dec 2019 11:25:54	U	SMPL
CCB10 - 1	CCB10	227	-0.0065 ✓		7470A	PPB	12 Dec 2019 11:28:00	U	SMPL
K6204-16 - 1	K072-AB-WC-1	367	0.0288 ✓		7470A	PPB	12 Dec 2019 11:30:07	U	SMPL
K6205-08 - 1	K165-WC-1	329	0.0192 ✓		7470A	PPB	12 Dec 2019 11:32:13	U	SMPL
K6205-09 - 1	K165-WC-2	0	-0.0638 ✓		7470A	PPB	12 Dec 2019 11:34:19	U	SMPL
PB125401BL - 1	PBW	2	-0.0633 ✓		7470A	PPB	12 Dec 2019 11:36:25	U	SMPL
PB125401BS - 1	LCSW	16503	4.1008 ✓		7470A	PPB	12 Dec 2019 11:38:30	U	SMPL
K6197-04 - 1	WC-S	-12	-0.0668 ✓		7470A	PPB	12 Dec 2019 11:40:37	U	SMPL
K6197-04DUP - 1	WC-SDUP	132	-0.0305 ✓		7470A	PPB	12 Dec 2019 11:42:42	U	SMPL
K6197-04MS - 1	WC-SMS	14417	3.5744 ✓		7470A	PPB	12 Dec 2019 11:51:32	U	SMPL
K6197-04MSD - 1	WC-SMSD	15054	3.7352 ✓		7470A	PPB	12 Dec 2019 11:57:10	U	SMPL
K6242-09 - 1	SB-01-COMP	467	0.0541 ✓		7470A	PPB	12 Dec 2019 11:59:17	U	SMPL
CCV11 - 1	CCV11	20883	5.2061 ✓		7470A	PPB	12 Dec 2019 12:01:23	U	SMPL
CCB11 - 1	CCB11	73	-0.0454 ✓		7470A	PPB	12 Dec 2019 12:03:29	U	SMPL
K6242-10 - 1	SB-02-COMP	319	0.0167 ✓		7470A	PPB	12 Dec 2019 12:05:36	U	SMPL
K6242-11 - 1	SB-03-COMP	331	0.0197 ✓		7470A	PPB	12 Dec 2019 12:07:43	U	SMPL
K6242-12 - 1	SB-04-COMP	335	0.0207 ✓		7470A	PPB	12 Dec 2019 12:09:49	U	SMPL
K6247-03 - 1	RBR200059	260	0.0018 ✓		7470A	PPB	12 Dec 2019 12:11:56	U	SMPL
K6247-06 - 1	RT3465	256	0.0008 ✓		7470A	PPB	12 Dec 2019 12:14:02	U	SMPL
K6204-14LX5 - 1		-1	-0.0640 ✓		7470A	PPB	12 Dec 2019 12:16:10	U	SMPL
K6197-04LX5 - 1		34	-0.0552 ✓		7470A	PPB	12 Dec 2019 12:18:17	U	SMPL
PB125400TB - 1	PB125341TB	101	-0.0383 ✓		7470A	PPB	12 Dec 2019 12:20:24	U	SMPL
PB125401TB - 1	PB125376TB	100	-0.0386 ✓		7470A	PPB	12 Dec 2019 12:22:32	U	SMPL
CCV12 - 1	CCV12	19098	4.7557 ✓		7470A	PPB	12 Dec 2019 12:24:39	U	SMPL
CCB12 - 1	CCB12	87	-0.0418 ✓		7470A	PPB	12 Dec 2019 12:26:45	U	SMPL