


LB106736

INSTRUMENT ID W1

7470A

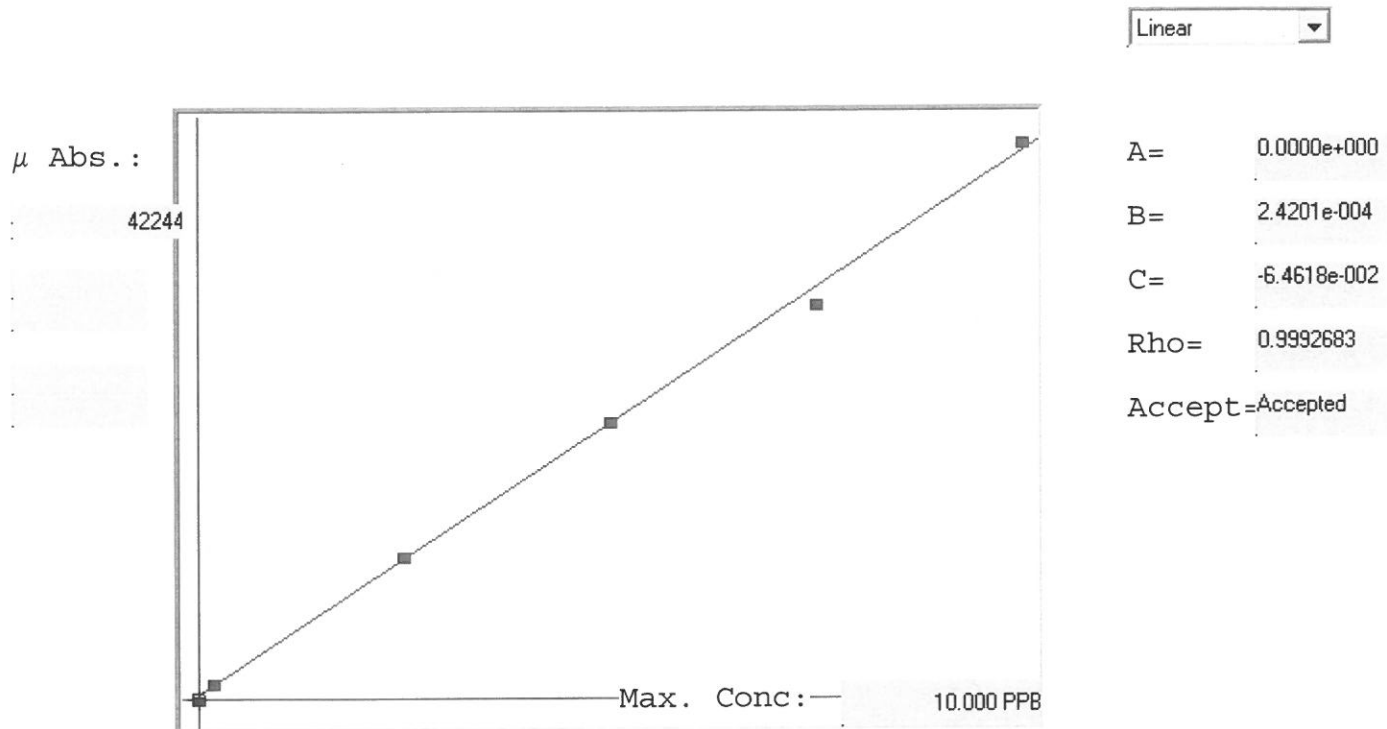

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.030	-0.030	144	0.000	144				
0.2	0.200	0.231	0.031	1222	0.0 %	1222				
2.5	2.500	2.576	0.076	10912	0.0 %	10912				
5.0	5.000	5.053	0.053	21145	0.0 %	21145				
7.5	7.500	7.211	-0.289	30061	0.0 %	30061				
10.0	10.000	10.159	0.159	42244	0.0 %	42244				

Ib106736 INSTRUMENT ID CV1

Method: 7470A		Operator: Admin		Date of Analysis: 13 Dec 2019 09:59:35				
Sample ID	Extended ID	µ Abs	Conc	Std Conc	Method	Units	Date	Type
0.0 - 1	S0.0	144	-	0.0000	7470A	PPB	13 Dec 2019 10:00:04	S Std
0.2 - 1	S0.2	1222	-	0.2000	7470A	PPB	13 Dec 2019 10:02:12	S Std
2.5 - 1	S2.5	10912	-	2.5000	7470A	PPB	13 Dec 2019 10:04:21	S Std
5.0 - 1	S5.0	21145	-	5.0000	7470A	PPB	13 Dec 2019 10:06:28	S Std
7.5 - 1	S7.5	30061	-	7.5000	7470A	PPB	13 Dec 2019 10:08:36	S Std
10.0 - 1	S10.0	42244	-	10.0000	7470A	PPB	13 Dec 2019 10:13:38	S Std
ICV28 - 1	ICV28	16515	3.9323	-	7470A	PPB	13 Dec 2019 10:16:23	U SMPL
ICB28 - 1	ICB28	7	-0.0629	-	7470A	PPB	13 Dec 2019 10:18:28	U SMPL
CCV16 - 1	CCV16	20887	4.9903	-	7470A	PPB	13 Dec 2019 10:20:34	U SMPL
CCB16 - 1	CCB16	0	-0.0646	-	7470A	PPB	13 Dec 2019 10:22:40	U SMPL
CRA - 1	CRA	1199	0.2256	-	7470A	PPB	13 Dec 2019 10:24:46	U SMPL
HighStd - 1	HighStd	42609	10.2474	-	7470A	PPB	13 Dec 2019 10:26:53	U SMPL
ChkStd - 1	ChkStd	28212	6.7631	-	7470A	PPB	13 Dec 2019 10:34:27	U SMPL
PB125426BL - 1	PBW	-5	-0.0658	-	7470A	PPB	13 Dec 2019 10:36:34	U SMPL
PB125426BS - 1	LCSW	16780	3.9964	-	7470A	PPB	13 Dec 2019 10:38:41	U SMPL
K5664-05 - 1	02-03-08-09-10-11-12-COMP	5	-0.0634	-	7470A	PPB	13 Dec 2019 10:40:48	U SMPL
K5674-01 - 1	OILY-WATER-DRUM	8	-0.0624	-	7470A	PPB	13 Dec 2019 10:42:56	U SMPL
K5674-02 - 1	OILY-WATER-DRUM	43	-0.0542	-	7470A	PPB	13 Dec 2019 10:45:03	U SMPL
K5674-02DUP - 1	OILY-WATER-DRUMDUP	41	-0.0547	-	7470A	PPB	13 Dec 2019 10:47:12	U SMPL
K5674-02MS - 1	OILY-WATER-DRUMMS	15235	3.6225	-	7470A	PPB	13 Dec 2019 10:49:18	U SMPL
CCV17 - 1	CCV17	21337	5.0992	-	7470A	PPB	13 Dec 2019 10:51:24	U SMPL
CCB17 - 1	CCB17	21	-0.0595	-	7470A	PPB	13 Dec 2019 10:53:31	U SMPL
K5674-02MSD - 1	OILY-WATER-DRUMMSD	15532	3.6944	-	7470A	PPB	13 Dec 2019 10:55:37	U SMPL
PB125428BL - 1	PBW	4	-0.0636	-	7470A	PPB	13 Dec 2019 10:57:43	U SMPL
PB125428BS - 1	LCSW	15914	3.7868	-	7470A	PPB	13 Dec 2019 10:59:50	U SMPL
K5664-04 - 1	02-03-08-09-10-11-12-COMP	59	-0.0503	-	7470A	PPB	13 Dec 2019 11:01:56	U SMPL
K5674-01 - 1	OILY-WATER-DRUM	37	-0.0557	-	7470A	PPB	13 Dec 2019 11:04:03	U SMPL
K6235-01 - 1	MW-08	66	-0.0486	-	7470A	PPB	13 Dec 2019 11:06:10	U SMPL
K6235-02 - 1	MW-07	23	-0.0591	-	7470A	PPB	13 Dec 2019 11:08:18	U SMPL
K6235-03 - 1	MW-03	1064	0.1929	-	7470A	PPB	13 Dec 2019 11:10:26	U SMPL
K6235-04 - 1	DUP	-6	-0.0661	-	7470A	PPB	13 Dec 2019 11:12:34	U SMPL
K6235-04DUP - 1	DUPDUP	68	-0.0482	-	7470A	PPB	13 Dec 2019 11:14:40	U SMPL
CCV18 - 1	CCV18	19556	4.6682	-	7470A	PPB	13 Dec 2019 11:16:46	U SMPL
CCB18 - 1	CCB18	-33	-0.0726	-	7470A	PPB	13 Dec 2019 11:18:52	U SMPL
K6235-04MS - 1	DUPMS	14529	3.4516	-	7470A	PPB	13 Dec 2019 11:23:23	U SMPL
K6235-04MSD - 1	DUPMSD	14580	3.4640	-	7470A	PPB	13 Dec 2019 11:25:29	U SMPL
K5674-02LX5 - 1		-7	-0.0663	-	7470A	PPB	13 Dec 2019 11:27:35	U SMPL
K6235-04LX5 - 1		16	-0.0607	-	7470A	PPB	13 Dec 2019 11:29:42	U SMPL
PB125426TB - 1	PB125415TB	0	-0.0646	-	7470A	PPB	13 Dec 2019 11:31:49	U SMPL
CCV19 - 1	CCV19	20622	4.9262	-	7470A	PPB	13 Dec 2019 11:33:36	U SMPL
CCB19 - 1	CCB19	6	-0.0632	-	7470A	PPB	13 Dec 2019 11:35:43	U SMPL

67
12/13/19