

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

12/13/2019 14:58

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.968	0.0	0.105	
ICB1	0.013	0.0	0.009	
CCV1	0.964	0.0	0.105	
CCB1	0.013	0.0	0.009	
PB125419BL	0.011	0.0	0.008	
PB125419BS	0.940	0.0	0.102	
K6258-01	0.006	0.0	0.008	
K6258-01DUP	0.006	0.0	0.008	
K6258-01MS	0.961	0.0	0.104	
K6258-01MSD	0.875	0.0	0.096	
K6258-02	0.008	0.0	0.008	
CCV2	0.980	0.0	0.106	
CCB2	0.011	0.0	0.008	

N	13
Mean	0.443
SD	0.4875
CV%	110.13

Aquakem v. 7.2AQ1

Results from time period:

Fri Dec 13 14:02:25 2019

Fri Dec 13 14:54:15 2019

A

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0531	mg/l	12/13/2019 14:02:25	
0.1PPM	A	Phenolics-	P	0.1031	mg/l	12/13/2019 14:02:26	
0.25PPM	A	Phenolics-	P	0.2547	mg/l	12/13/2019 14:02:27	
0.50PPM	A	Phenolics-	P	0.4893	mg/l	12/13/2019 14:02:28	
1.0PPM	A	Phenolics-	P	0.9959	mg/l	12/13/2019 14:02:29	
2.0PPM	A	Phenolics-	P	2.0039	mg/l	12/13/2019 14:02:30	
ICV1	S	Phenolics-	P	0.9678	mg/l	12/13/2019 14:32:25	
ICB1	S	Phenolics-	P	0.0128	mg/l	12/13/2019 14:32:26	
CCV1	S	Phenolics-	P	0.9636	mg/l	12/13/2019 14:32:27	
CCB1	S	Phenolics-	P	0.0126	mg/l	12/13/2019 14:32:28	
PB125419BL	S	Phenolics-	P	0.0113	mg/l	12/13/2019 14:32:29	
PB125419BS	S	Phenolics-	P	0.9399	mg/l	12/13/2019 14:32:30	
K6258-01	S	Phenolics-	P	0.0058	mg/l	12/13/2019 14:32:31	
K6258-01DUP	S	Phenolics-	P	0.0059	mg/l	12/13/2019 14:32:32	
K6258-01MS	S	Phenolics-	P	0.961	mg/l	12/13/2019 14:32:33	
K6258-01MSD	S	Phenolics-	P	0.8752	mg/l	12/13/2019 14:32:34	
K6258-02	S	Phenolics-	P	0.0076	mg/l	12/13/2019 14:32:35	
CCV2	S	Phenolics-	P	0.9802	mg/l	12/13/2019 14:54:14	
CCB2	S	Phenolics-	P	0.0111	mg/l	12/13/2019 14:54:15	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AL

Instrument ID : Konelab

12/13/2019 14:04


Test Phenolics-

Accepted 12/13/2019 14:04

Factor 9.889
Bias 0.007

Coeff. of det. 0.999932

Errors

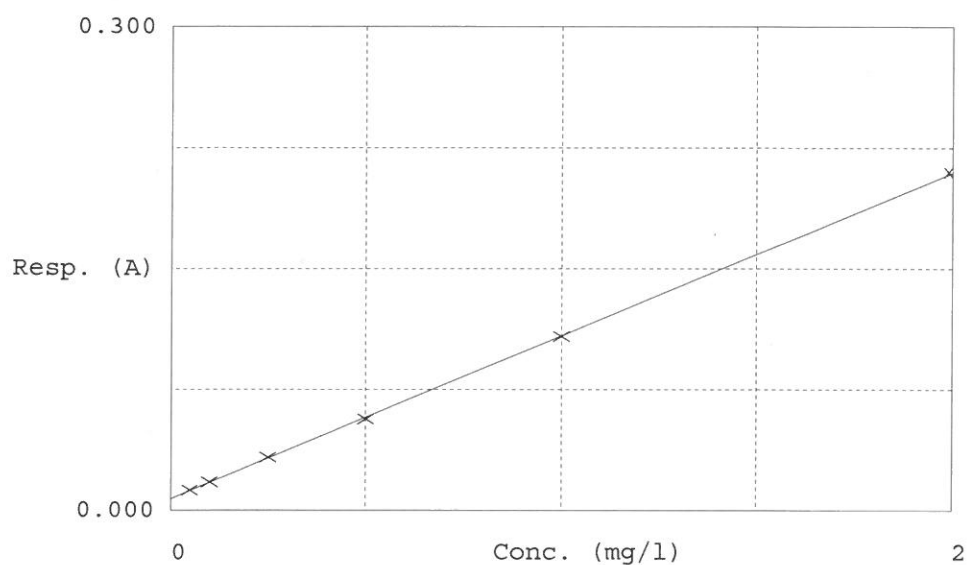

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.013	0.0531	0.0500	
2	Phenol-2	0.018	0.1031	0.1000	
3	Phenol-2	0.033	0.2547	0.2500	
4	Phenol-2	0.057	0.4893	0.5000	
5	Phenol-2	0.108	0.9959	1.0000	
6	Phenol-2	0.210	2.0039	2.0000	