


LB106753
INSTRUMENT ID W1

7470A

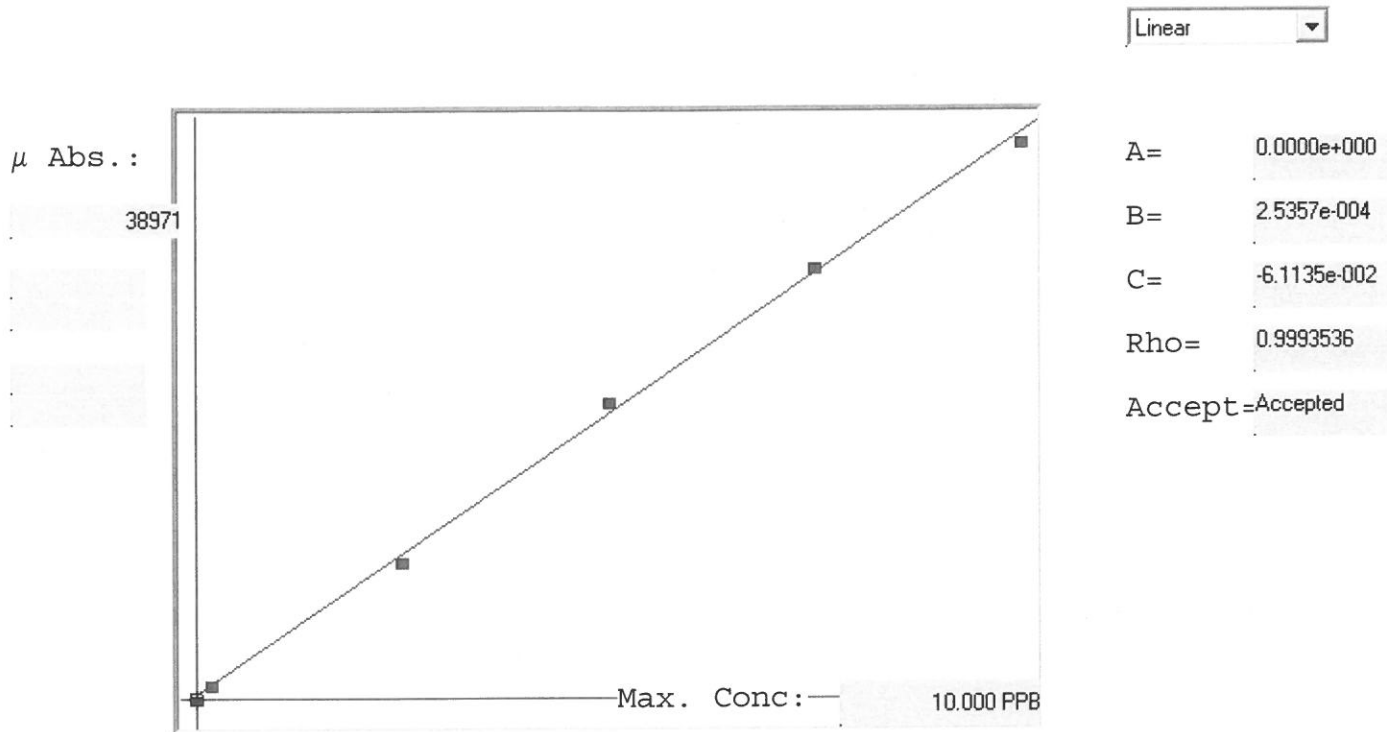

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.035	-0.035	102	0.000	102				
0.2	0.200	0.195	-0.005	1010	0.0 %	1010				
2.5	2.500	2.387	-0.113	9653	0.0 %	9653				
5.0	5.000	5.210	0.210	20789	0.0 %	20789				
7.5	7.500	7.623	0.123	30303	0.0 %	30303				
10.0	10.000	9.821	-0.179	38971	0.0 %	38971				

Ib106736 INSTRUMENT ID CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Dec 2019 15:43:02

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	102	-	0.0000	7470A	PPB	13 Dec 2019 15:43:14	S	Std
0.2 - 1	50.2	1010	-	0.2000	7470A	PPB	13 Dec 2019 15:45:22	S	Std
2.5 - 1	52.5	9653	-	2.5000	7470A	PPB	13 Dec 2019 15:47:30	S	Std
5.0 - 1	55.0	20789	-	5.0000	7470A	PPB	13 Dec 2019 15:49:37	S	Std
7.5 - 1	57.5	30303	-	7.5000	7470A	PPB	13 Dec 2019 15:54:39	S	Std
10.0 - 1	510.0	38971	-	10.0000	7470A	PPB	13 Dec 2019 15:56:45	S	Std
ICV29 - 1	ICV29	16957	4.2386	-	7470A	PPB	13 Dec 2019 16:12:29	U	SMPL
ICB29 - 1	ICB29	8	-0.0591	-	7470A	PPB	13 Dec 2019 16:14:35	U	SMPL
CCV20 - 1	CCV20	20614	5.1659	-	7470A	PPB	13 Dec 2019 16:16:41	U	SMPL
CCB20 - 1	CCB20	11	-0.0583	-	7470A	PPB	13 Dec 2019 16:18:48	U	SMPL
CRA - 1	CRA	977	0.1866	-	7470A	PPB	13 Dec 2019 16:20:54	U	SMPL
HighStd - 1	HighStd	40165	10.1234	-	7470A	PPB	13 Dec 2019 16:23:00	U	SMPL
ChkStd - 1	ChkStd	29573	7.4376	-	7470A	PPB	13 Dec 2019 16:25:06	U	SMPL
PB125468BL - 1	PBW	-34	-0.0698	-	7470A	PPB	13 Dec 2019 16:27:13	U	SMPL
PB125468BS - 1	LCSW	17334	4.3342	-	7470A	PPB	13 Dec 2019 16:29:20	U	SMPL
K6110-04 - 1	HD-02-121219	-11	-0.0639	-	7470A	PPB	13 Dec 2019 16:31:27	U	SMPL
K6110-04DUP - 1	HD-02-121219DUP	30	-0.0535	-	7470A	PPB	13 Dec 2019 16:33:35	U	SMPL
K6110-04MS - 1	HD-02-121219MS	15677	3.9141	-	7470A	PPB	13 Dec 2019 16:35:42	U	SMPL
K6110-04MSD - 1	HD-02-121219MSD	15846	3.9569	-	7470A	PPB	13 Dec 2019 16:37:50	U	SMPL
K6265-04 - 1	TP-1A-S	56	-0.0469	-	7470A	PPB	13 Dec 2019 16:39:56	U	SMPL
CCV21 - 1	CCV21	20846	5.2248	-	7470A	PPB	13 Dec 2019 16:42:02	U	SMPL
CCB21 - 1	CCB21	7	-0.0594	-	7470A	PPB	13 Dec 2019 16:44:09	U	SMPL
K6265-08 - 1	TP-1A-D	38	-0.0515	-	7470A	PPB	13 Dec 2019 16:46:15	U	SMPL
K6274-03 - 1	T2-COMP	-4	-0.0621	-	7470A	PPB	13 Dec 2019 16:48:21	U	SMPL
K6283-01 - 1	SOIL-CUTTINGS	61	-0.0457	-	7470A	PPB	13 Dec 2019 16:50:28	U	SMPL
K6110-04LX5 - 1		8	-0.0591	-	7470A	PPB	13 Dec 2019 16:52:34	U	SMPL
PB125468TB - 1	PB125418TB	50	-0.0485	-	7470A	PPB	13 Dec 2019 16:54:41	U	SMPL
CCV22 - 1	CCV22	21173	5.3077	-	7470A	PPB	13 Dec 2019 16:56:48	U	SMPL
CCB22 - 1	CCB22	-18	-0.0657	-	7470A	PPB	13 Dec 2019 16:58:56	U	SMPL