


LB106788
INSTRUMENT ID CN1

7471B

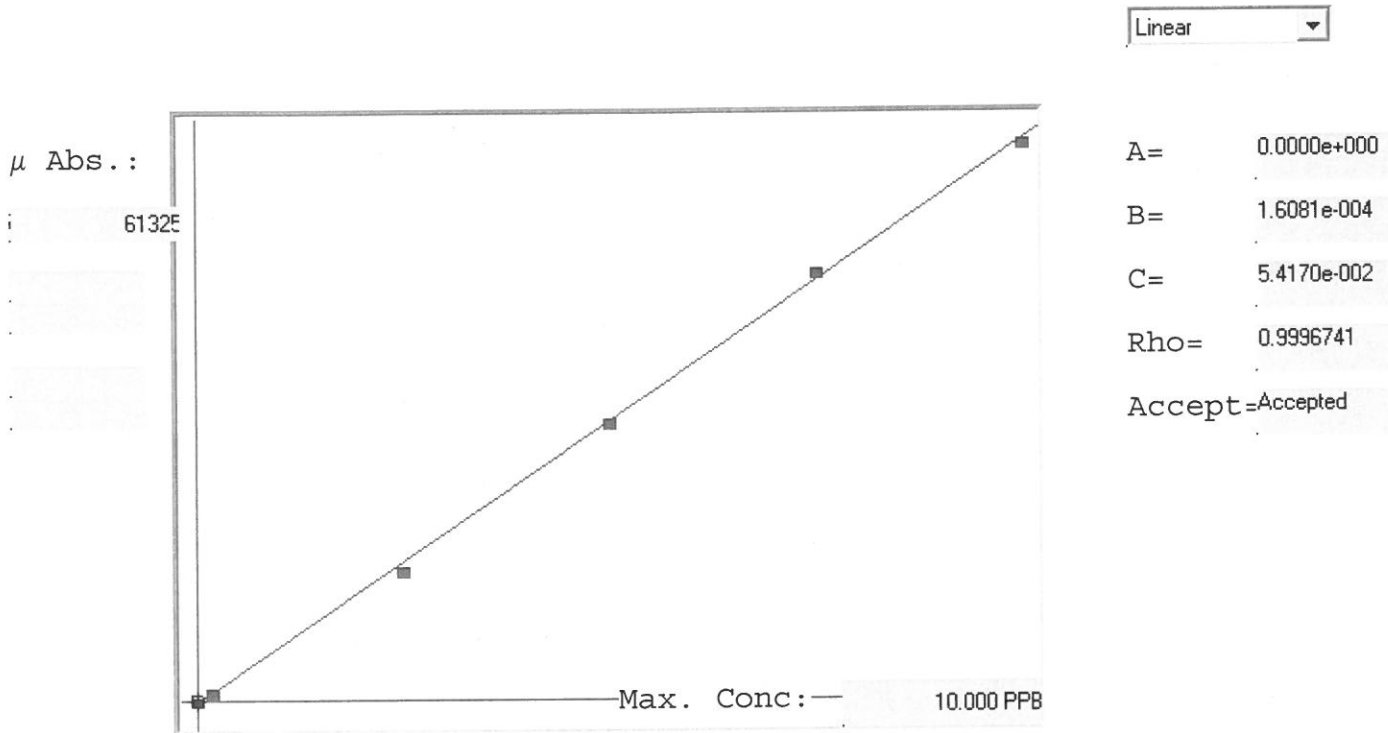

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.055	0.055	7	0.000	7				
0.2	0.200	0.217	0.017	1011	0.0 %	1011				
2.5	2.500	2.372	-0.128	14415	0.0 %	14415				
5.0	5.000	4.978	-0.022	30618	0.0 %	30618				
7.5	7.500	7.662	0.162	47305	0.0 %	47305				
10.0	10.000	9.916	-0.084	61325	0.0 %	61325				

Ib106788 INSTRUMENT ID CV1

Method: 7471B		Operator: Admin		Date of Analysis: 17 Dec 2019 07:28:14					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	80.0	7	-	0.0000	7471B	PPB	17 Dec 2019 07:30:19	S	Std
0.2 - 1	80.2	1011	-	0.2000	7471B	PPB	17 Dec 2019 07:32:37	S	Std
2.5 - 1	82.5	14415	-	2.5000	7471B	PPB	17 Dec 2019 07:34:54	S	Std
5.0 - 1	85.0	30618	-	5.0000	7471B	PPB	17 Dec 2019 07:37:11	S	Std
7.5 - 1	87.5	47305	-	7.5000	7471B	PPB	17 Dec 2019 07:42:55	S	Std
10.0 - 1	810.0	61325	-	10.0000	7471B	PPB	17 Dec 2019 07:51:23	S	Std
ICV32 - 1	ICV32	22564	3.6828 ✓	-	7471B	PPB	17 Dec 2019 07:54:10	U	SMPL
ICB32 - 1	ICB32	11	0.0559 ✓	-	7471B	PPB	17 Dec 2019 07:57:14	U	SMPL
CCV29 - 1	CCV29	30838	5.0134 ✓	-	7471B	PPB	17 Dec 2019 07:59:29	U	SMPL
CCB29 - 1	CCB29	-21	0.0508 ✓	-	7471B	PPB	17 Dec 2019 08:01:44	U	SMPL
CRA - 1	CRA	1053	0.2235 ✓	-	7471B	PPB	17 Dec 2019 08:06:04	U	SMPL
HighStd - 1	HighStd	57859	9.3587 ✓	-	7471B	PPB	17 Dec 2019 08:08:19	U	SMPL
ChkStd - 1	ChkStd	43652	7.0741 ✓	-	7471B	PPB	17 Dec 2019 08:10:35	U	SMPL
PB125508BL - 1	PBS	-52	0.0458 ✓	-	7471B	PPB	17 Dec 2019 08:12:53	U	SMPL
PB125508BS - 1	LCSS	22852	3.7291 ✓	-	7471B	PPB	17 Dec 2019 08:15:10	U	SMPL
K6113-06 - 1	OR-02-121319	1233	0.2525 ✓	-	7471B	PPB	17 Dec 2019 08:17:26	U	SMPL
K6113-06DUP - 1	OR-02-121319DUP	1271	0.2586 ✓	-	7471B	PPB	17 Dec 2019 08:21:12	U	SMPL
K6113-06MS - 1	OR-02-121319MS	23277	3.7975 ✓	-	7471B	PPB	17 Dec 2019 08:23:29	U	SMPL
K6113-06MSD - 1	OR-02-121319MSD	22892	3.7355 ✓	-	7471B	PPB	17 Dec 2019 08:25:46	U	SMPL
K6117-04 - 1	TR-05-121319	21778	3.5564 ✓	-	7471B	PPB	17 Dec 2019 08:28:01	U	SMPL
CCV30 - 1	CCV30	30458	4.9523 ✓	-	7471B	PPB	17 Dec 2019 08:30:17	U	SMPL
CCB30 - 1	CCB30	0	0.0542 ✓	-	7471B	PPB	17 Dec 2019 08:32:33	U	SMPL
K6118-06 - 1	SU-03-121319	32378	5.2610 ✓	-	7471B	PPB	17 Dec 2019 08:34:48	U	SMPL
K6292-01 - 1	72-11999	11876	1.9640 ✓	-	7471B	PPB	17 Dec 2019 08:37:04	U	SMPL
K6294-01 - 1	TP-1	1018	0.2179 ✓	-	7471B	PPB	17 Dec 2019 08:39:20	U	SMPL
K6294-04 - 1	TP-2	3041	0.5432 ✓	-	7471B	PPB	17 Dec 2019 08:41:35	U	SMPL
K6299-02 - 1	SHORE-RD-BH-01	11341	1.8780 ✓	-	7471B	PPB	17 Dec 2019 08:43:52	U	SMPL
K6299-04 - 1	SHORE-RD-BH-02B	6466	1.0940 ✓	-	7471B	PPB	17 Dec 2019 08:46:08	U	SMPL
K6299-06 - 1	SHORE-RD-BH-02	2702	0.4887 ✓	-	7471B	PPB	17 Dec 2019 08:48:25	U	SMPL
K6299-08 - 1	SHORE-RD-BH-03	2272	0.4195 ✓	-	7471B	PPB	17 Dec 2019 08:50:42	U	SMPL
K6299-10 - 1	SHORE-RD-BH-04	5022	0.8618 ✓	-	7471B	PPB	17 Dec 2019 08:53:00	U	SMPL
K6310-03 - 1	SP-01	4488	0.7759 ✓	-	7471B	PPB	17 Dec 2019 08:55:15	U	SMPL
CCV31 - 1	CCV31	29900	4.8625 ✓	-	7471B	PPB	17 Dec 2019 08:57:31	U	SMPL
CCB31 - 1	CCB31	32	0.0593 ✓	-	7471B	PPB	17 Dec 2019 08:59:46	U	SMPL
K6113-06LX5 - 1		259	0.0958 ✓	-	7471B	PPB	17 Dec 2019 09:02:01	U	SMPL
CCV32 - 1	CCV32	28642	4.6602 ✓	-	7471B	PPB	17 Dec 2019 09:04:17	U	SMPL
CCB32 - 1	CCB32	-5	0.0534 ✓	-	7471B	PPB	17 Dec 2019 09:06:32	U	SMPL