


LB106844
INSTRUMENT ID 001

7471B

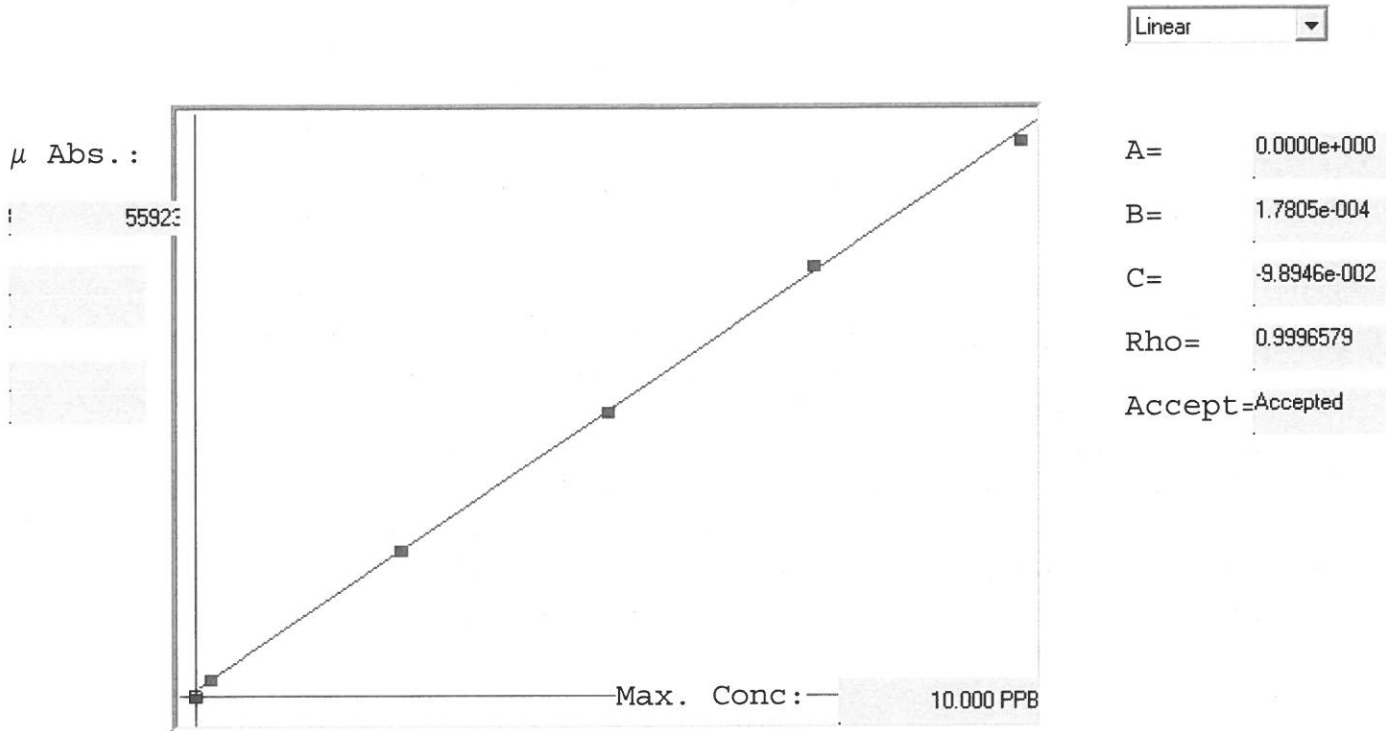

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.097	-0.097	9	0.000	9				
0.2	0.200	0.217	0.017	1776	0.0 %	1776				
2.5	2.500	2.551	0.051	14886	0.0 %	14886				
5.0	5.000	5.019	0.019	28745	0.0 %	28745				
7.5	7.500	7.651	0.151	43530	0.0 %	43530				
10.0	10.000	9.858	-0.142	55923	0.0 %	55923				

LB106844 INSTRUMENT ID CV1

Method: 7471B		Operator: Admin		Date of Analysis: 19 Dec 2019 07:41:59				
Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50.0	9	-	0.00007471B	PPB	19 Dec 2019 07:48:43	S	Std
0.2 - 1	50.2	1776	-	0.20007471B	PPB	19 Dec 2019 07:51:00	S	Std
2.5 - 1	52.5	14886	-	2.50007471B	PPB	19 Dec 2019 07:53:17	S	Std
5.0 - 1	56.0	28745	-	5.00007471B	PPB	19 Dec 2019 07:55:34	S	Std
7.5 - 1	57.5	43530	-	7.50007471B	PPB	19 Dec 2019 07:57:51	S	Std
10.0 - 1	510.0	55923	-	10.00007471B	PPB	19 Dec 2019 08:01:43	S	Std
ICV35 - 1	ICV35	22752	3.9520	-7471B	PPB	19 Dec 2019 08:06:04	U	SMPL
ICB35 - 1	ICB35	8	-0.0975	-7471B	PPB	19 Dec 2019 08:08:19	U	SMPL
CCV42 - 1	CCV42	28968	5.0588	-7471B	PPB	19 Dec 2019 08:10:35	U	SMPL
CCB42 - 1	CCB42	-12	-0.1011	-7471B	PPB	19 Dec 2019 08:12:50	U	SMPL
CRA - 1	CRA	1503	0.1687	-7471B	PPB	19 Dec 2019 08:20:00	U	SMPL
HighStd - 1	HighStd	54708	9.6417	-7471B	PPB	19 Dec 2019 08:22:15	U	SMPL
ChkStd - 1	ChkStd	38318	6.7235	-7471B	PPB	19 Dec 2019 08:24:31	U	SMPL
PB125582BL - 1	PBS	6	-0.0979	-7471B	PPB	19 Dec 2019 08:26:48	U	SMPL
PB125582BS - 1	LCSS	22725	3.9472	-7471B	PPB	19 Dec 2019 08:29:04	U	SMPL
K6107-01 - 1	HR-06-121819	2527	0.3510	-7471B	PPB	19 Dec 2019 08:31:21	U	SMPL
K6317-07 - 1	178K-WC1	1067	0.0910	-7471B	PPB	19 Dec 2019 08:33:37	U	SMPL
K6317-07DUP - 1	178K-WC1DUP	1069	0.0914	-7471B	PPB	19 Dec 2019 08:35:54	U	SMPL
K6317-07MS - 1	178K-WC1MS	21167	3.6698	-7471B	PPB	19 Dec 2019 08:38:11	U	SMPL
K6317-07MSD - 1	178K-WC1MSD	20578	3.5649	-7471B	PPB	19 Dec 2019 08:40:26	U	SMPL
CCV43 - 1	CCV43	28895	5.0458	-7471B	PPB	19 Dec 2019 08:42:42	U	SMPL
CCB43 - 1	CCB43	11	-0.0970	-7471B	PPB	19 Dec 2019 08:44:57	U	SMPL
K6317-08 - 1	178K-WC2	767	0.0376	-7471B	PPB	19 Dec 2019 08:47:12	U	SMPL
K6318-07 - 1	X089-WC-1	3421	0.5102	-7471B	PPB	19 Dec 2019 08:49:28	U	SMPL
K6318-08 - 1	X089-WC-2	555	-0.0001	-7471B	PPB	19 Dec 2019 08:51:43	U	SMPL
K6325-01 - 1	RT-3860	1732	0.2094	-7471B	PPB	19 Dec 2019 08:53:59	U	SMPL
K6325-04 - 1	RT-3425	599	0.0077	-7471B	PPB	19 Dec 2019 08:56:15	U	SMPL
K6327-01 - 1	C-1	1097	0.0964	-7471B	PPB	19 Dec 2019 08:58:32	U	SMPL
K6328-01 - 1	OIL-SAMPLE-2-BG24	443	-0.0201	-7471B	PPB	19 Dec 2019 09:00:49	U	SMPL
K6329-01 - 1	121619-CA-COMP	3988	0.6111	-7471B	PPB	19 Dec 2019 09:03:06	U	SMPL
K6333-04 - 1	TP-1A-COMP	1921	0.2431	-7471B	PPB	19 Dec 2019 09:05:23	U	SMPL
K6350-01 - 1	RO-1-3	3020	0.4388	-7471B	PPB	19 Dec 2019 09:07:39	U	SMPL
CCV44 - 1	CCV44	29370	5.1303	-7471B	PPB	19 Dec 2019 09:09:55	U	SMPL
CCB44 - 1	CCB44	17	-0.0959	-7471B	PPB	19 Dec 2019 09:12:10	U	SMPL
K6357-01 - 1	PF-01	469	-0.0154	-7471B	PPB	19 Dec 2019 09:14:26	U	SMPL
K6357-02 - 1	PF-02	442	-0.0202	-7471B	PPB	19 Dec 2019 09:16:41	U	SMPL
K6357-03 - 1	PF-03	401	-0.0275	-7471B	PPB	19 Dec 2019 09:18:57	U	SMPL
K6357-04 - 1	PF-04	431	-0.0222	-7471B	PPB	19 Dec 2019 09:21:13	U	SMPL
K6357-05 - 1	PF-05	379	-0.0315	-7471B	PPB	19 Dec 2019 09:23:30	U	SMPL
K6360-01 - 1	1FT-TP	4259	0.6594	-7471B	PPB	19 Dec 2019 09:25:46	U	SMPL
K6370-01 - 1	TP1-3	29046	5.0726	-7471B	PPB	19 Dec 2019 09:28:03	U	SMPL
K6370-03 - 1	TP1-6	10281	1.7316	-7471B	PPB	19 Dec 2019 09:30:21	U	SMPL
K6370-05 - 1	TP2-3	12937	2.2045	-7471B	PPB	19 Dec 2019 09:32:39	U	SMPL
K6370-07 - 1	TP2-6	14987	2.5695	-7471B	PPB	19 Dec 2019 09:34:55	U	SMPL
CCV45 - 1	CCV45	29504	5.1542	-7471B	PPB	19 Dec 2019 09:37:11	U	SMPL
CCB45 - 1	CCB45	-15	-0.1016	-7471B	PPB	19 Dec 2019 09:39:26	U	SMPL
K6317-07LX5 - 1		218	-0.0601	-7471B	PPB	19 Dec 2019 09:41:42	U	SMPL
CCV46 - 1	CCV46	28857	5.0390	-7471B	PPB	19 Dec 2019 09:43:58	U	SMPL
CCB46 - 1	CCB46	-23	-0.1030	-7471B	PPB	19 Dec 2019 09:46:13	U	SMPL