

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Dk

Instrument ID : Konelab

12/20/2019 15:55

Test: ^{Residue} ~~Total~~ CN

Sample Id	Result ^{mg/L}	Dil. 1 +	Response	Errors
ICV1	95.167	0.0	0.111	
ICB1	0.955	0.0	0.002	
CCV1	241.254	0.0	0.279	
CCB1	0.763	0.0	0.002	
PB125649BL	0.659	0.0	0.002	
K6107-05	0.631	0.0	0.002	
K6107-05DUP	0.521	0.0	0.002	
PB125646BL	0.584	0.0	0.002	
K6363-02	0.407	0.0	0.002	
K6363-02DUP	0.520	0.0	0.002	
CCV2	257.776	0.0	0.299	
CCB2	0.909	0.0	0.002	

N	12
Mean	50.012
SD	97.0934
CV%	194.14

LB106876

Aquakem v. 7.2AQ1

Results from time period:

Dk

Fri Dec 20 15:29:07 2019

Fri Dec 20 15:54:36 2019

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	REACTIVE CN	P	0.4224	µg/l	12/20/2019 11:16:59	
5.OPPBCN	A	REACTIVE CN	P	5.3867	µg/l	12/20/2019 11:17:00	
10PPBCN	A	REACTIVE CN	P	10.0821	µg/l	12/20/2019 11:17:01	
50PPBCN	A	REACTIVE CN	P	49.1459	µg/l	12/20/2019 11:17:02	
100PPBCN	A	REACTIVE CN	P	99.3198	µg/l	12/20/2019 11:17:03	
250PPBCN	A	REACTIVE CN	P	250.8544	µg/l	12/20/2019 11:17:04	
500PPBCN	A	REACTIVE CN	P	499.7887	µg/l	12/20/2019 11:17:05	
ICV1	S	REACTIVE CN	P	95.1671	µg/l	12/20/2019 15:29:07	
ICB1	S	REACTIVE CN	P	0.9553	µg/l	12/20/2019 15:29:08	
CCV1	S	REACTIVE CN	P	241.2541	µg/l	12/20/2019 15:29:09	
CCB1	S	REACTIVE CN	P	0.7632	µg/l	12/20/2019 15:29:10	
PB125649BL	S	REACTIVE CN	P	0.6593	µg/l	12/20/2019 15:29:11	
K6107-05	S	REACTIVE CN	P	0.6311	µg/l	12/20/2019 15:29:12	
K6107-05DUP	S	REACTIVE CN	P	0.5213	µg/l	12/20/2019 15:29:13	
PB125646BL	S	REACTIVE CN	P	0.5838	µg/l	12/20/2019 15:29:14	
K6363-02	S	REACTIVE CN	P	0.4075	µg/l	12/20/2019 15:54:33	
K6363-02DUP	S	REACTIVE CN	P	0.5203	µg/l	12/20/2019 15:54:34	
CCV2	S	REACTIVE CN	P	257.7764	µg/l	12/20/2019 15:54:35	
CCB2	S	REACTIVE CN	P	0.9088	µg/l	12/20/2019 15:54:36	

LB06876

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Dk

Instrument ID : Konelab

12/20/2019 14:37

Test ~~Total~~ ^{Reactive} CN


Accepted 12/20/2019 11:18

Factor 867.1

Bias 0.001

Coeff. of det. 0.999989

Errors

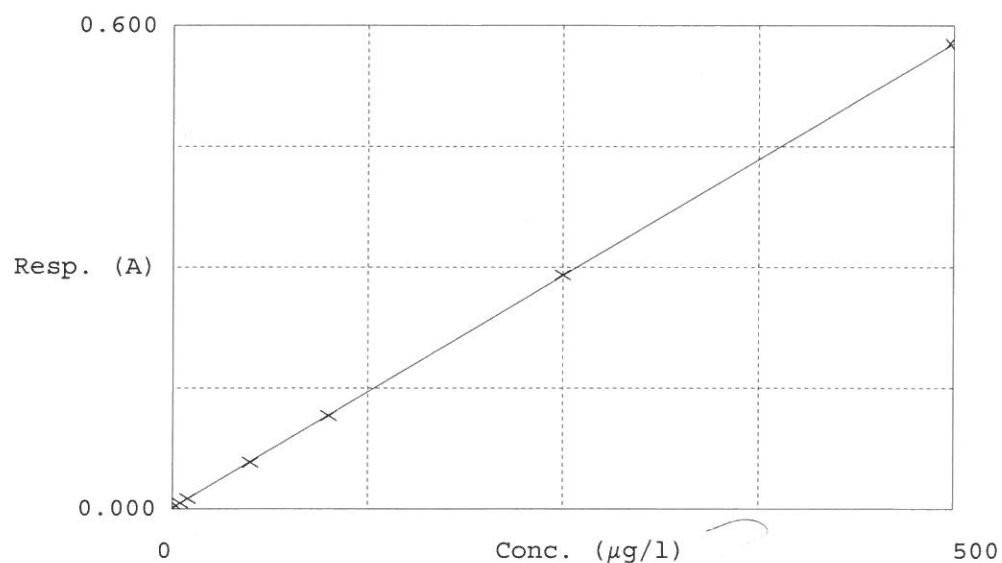

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.4224	0.0000	
2	5.0PPBCN	0.007	5.3867	5.0000	
3	10PPBCN	0.013	10.0821	10.0000	
4	50PPBCN	0.058	49.1459	50.0000	
5	100PPBCN	0.116	99.3198	100.0000	
6	250PPBCN	0.291	250.8544	250.0000	
7	500PPBCN	0.578	499.7887	500.0000	