


LB106888
INSTRUMENT ID 001

7470A

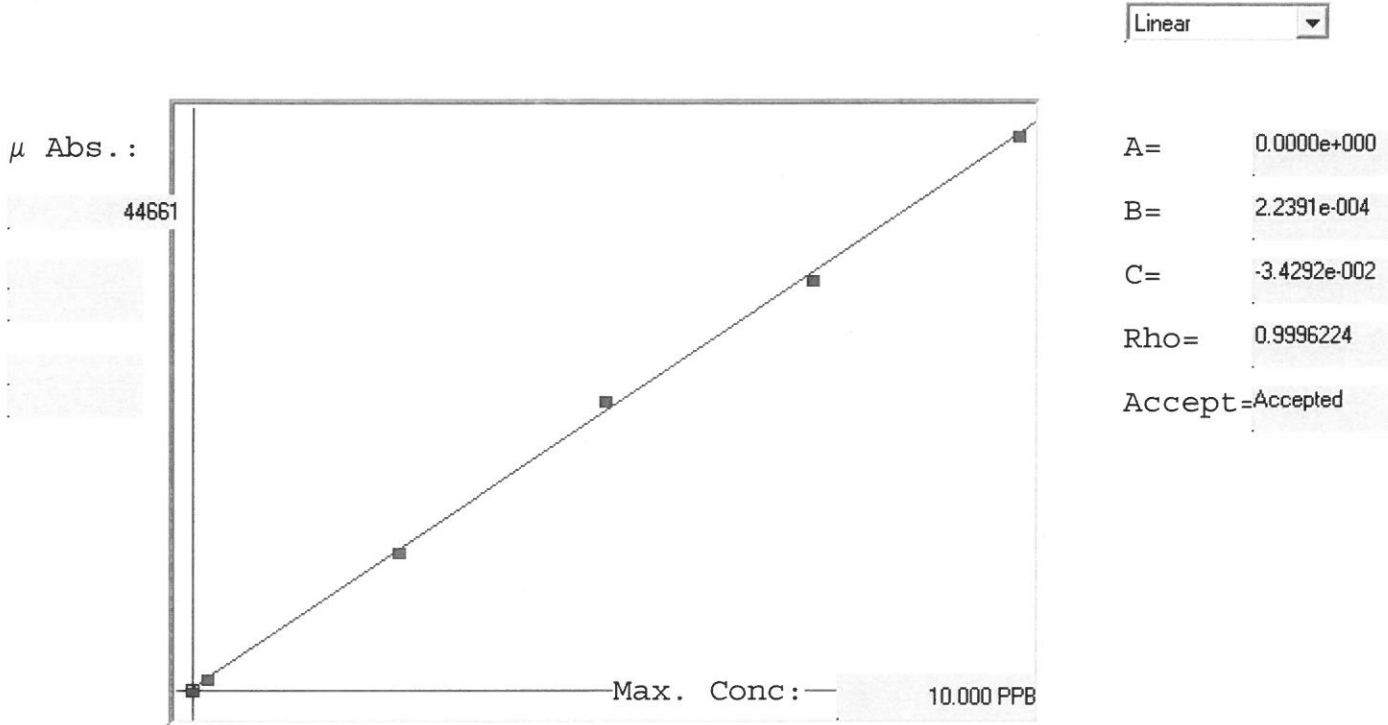

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.031	-0.031	16	0.000	16				
0.2	0.200	0.178	-0.022	946	0.0 %	946				
2.5	2.500	2.464	-0.036	11158	0.0 %	11158				
5.0	5.000	5.220	0.220	23466	0.0 %	23466				
7.5	7.500	7.403	-0.097	33216	0.0 %	33216				
10.0	10.000	9.966	-0.034	44661	0.0 %	44661				

LB106888 INSTRUMENT ID CV1

Method: 7470A		Operator: Admin		Date of Analysis: 23 Dec 2019 09:48:16									
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units		Date	Type	Type			
0.0 - 1	800	16	-	0.0000	7470A	PPB		23 Dec 2019 10:10:00	S	Std			
0.2 - 1	80.2	946	-	0.2000	7470A	PPB		23 Dec 2019 10:13:36	S	Std			
2.5 - 1	52.5	11158	-	2.5000	7470A	PPB		23 Dec 2019 10:15:44	S	Std			
5.0 - 1	55.0	23466	-	5.0000	7470A	PPB		23 Dec 2019 10:17:52	S	Std			
7.5 - 1	57.5	33216	-	7.5000	7470A	PPB		23 Dec 2019 10:20:00	S	Std			
10.0 - 1	510.0	44661	-	10.0000	7470A	PPB		23 Dec 2019 10:22:06	S	Std			
ICV38 - 1	ICV38	18274	4.0575		7470A	PPB		23 Dec 2019 10:30:41	U	SMPL			
ICB38 - 1	ICB38	0	-0.0343		7470A	PPB		23 Dec 2019 10:32:47	U	SMPL			
CCV59 - 1	CCV59	22036	4.8998		7470A	PPB		23 Dec 2019 10:34:53	U	SMPL			
CCB59 - 1	CCB59	-85	-0.0533		7470A	PPB		23 Dec 2019 10:37:00	U	SMPL			
CRA - 1	CRA	920	0.1717		7470A	PPB		23 Dec 2019 10:39:06	U	SMPL			
HighStd - 1	HighStd	44614	9.9553		7470A	PPB		23 Dec 2019 10:41:12	U	SMPL			
ChkStd - 1	ChkStd	29474	6.5653		7470A	PPB		23 Dec 2019 10:43:19	U	SMPL			
PB125654BL - 1	PBW	-233	-0.0865		7470A	PPB		23 Dec 2019 10:45:26	U	SMPL			
PB125654BS - 1	LCSW	17446	3.8721		7470A	PPB		23 Dec 2019 10:47:33	U	SMPL			
K6355-02 - 1	13954	-276	-0.0961		7470A	PPB		23 Dec 2019 10:49:41	U	SMPL			
K6363-02 - 1	T-2-CONTAINMENT-SUMP	-215	-0.0824		7470A	PPB		23 Dec 2019 10:51:50	U	SMPL			
K6363-02DUP - 1	T-2-CONTAINMENT-SUMPDUP	-182	-0.0750		7470A	PPB		23 Dec 2019 10:53:57	U	SMPL			
K6363-02MS - 1	T-2-CONTAINMENT-SUMPMMS	17938	3.9822		7470A	PPB		23 Dec 2019 10:56:05	U	SMPL			
K6363-02MSD - 1	T-2-CONTAINMENT-SUMPMMSD	18139	4.0273		7470A	PPB		23 Dec 2019 10:58:12	U	SMPL			
CCV60 - 1	CCV60	22195	4.9354		7470A	PPB		23 Dec 2019 11:00:18	U	SMPL			
CCB60 - 1	CCB60	-105	-0.0578		7470A	PPB		23 Dec 2019 11:02:24	U	SMPL			
PB125655BL - 1	PBW	-71	-0.0502		7470A	PPB		23 Dec 2019 11:04:30	U	SMPL			
PB125655BS - 1	LCSW	17549	3.8951		7470A	PPB		23 Dec 2019 11:06:37	U	SMPL			
K6117-09 - 1	TR-04-121919	-44	-0.0441		7470A	PPB		23 Dec 2019 11:08:43	U	SMPL			
K6117-09DUP - 1	TR-04-121919DUP	5	-0.0332		7470A	PPB		23 Dec 2019 11:10:49	U	SMPL			
K6117-09MS - 1	TR-04-121919MS	18331	4.0702		7470A	PPB		23 Dec 2019 11:12:56	U	SMPL			
K6117-09MSD - 1	TR-04-121919MSD	18452	4.0973		7470A	PPB		23 Dec 2019 11:15:04	U	SMPL			
PB125656BL - 1	PBW	12	-0.0316		7470A	PPB		23 Dec 2019 11:17:11	U	SMPL			
PB125656BS - 1	LCSW	17726	3.9348		7470A	PPB		23 Dec 2019 11:20:58	U	SMPL			
K6107-05 - 1	HR-06-121819	65	-0.0197		7470A	PPB		23 Dec 2019 11:23:06	U	SMPL			
K6107-05DUP - 1	HR-06-121819DUP	88	-0.0146		7470A	PPB		23 Dec 2019 11:25:12	U	SMPL			
CCV61 - 1	CCV61	22264	4.9509		7470A	PPB		23 Dec 2019 11:27:18	U	SMPL			
CCB61 - 1	CCB61	30	-0.0276		7470A	PPB		23 Dec 2019 11:29:25	U	SMPL			
K6107-05MS - 1	HR-06-121819MS	18144	4.0284		7470A	PPB		23 Dec 2019 11:31:31	U	SMPL			
K6107-05MSD - 1	HR-06-121819MSD	18172	4.0346		7470A	PPB		23 Dec 2019 11:33:37	U	SMPL			
K6370-02 - 1	TP1-3	23	-0.0291		7470A	PPB		23 Dec 2019 11:35:44	U	SMPL			
K6370-04 - 1	TP1-6	40	-0.0253		7470A	PPB		23 Dec 2019 11:37:50	U	SMPL			
K6370-06 - 1	TP2-3	62	-0.0204		7470A	PPB		23 Dec 2019 11:39:57	U	SMPL			
K6370-08 - 1	TP2-6	64	-0.0200		7470A	PPB		23 Dec 2019 11:42:04	U	SMPL			
K6386-02 - 1	STOCKPILE	48	-0.0235		7470A	PPB		23 Dec 2019 11:44:11	U	SMPL			
PB125658BL - 1	PBW	25	-0.0287		7470A	PPB		23 Dec 2019 11:46:19	U	SMPL			
PB125658BS - 1	LCSW	18561	4.1217		7470A	PPB		23 Dec 2019 11:48:27	U	SMPL			
K6355-01 - 1	30604	6	-0.0329		7470A	PPB		23 Dec 2019 11:50:34	U	SMPL			
CCV62 - 1	CCV62	23241	5.1697		7470A	PPB		23 Dec 2019 11:52:41	U	SMPL			
CCB62 - 1	CCB62	-24	-0.0397		7470A	PPB		23 Dec 2019 11:54:48	U	SMPL			
K6355-01DUP - 1	30604DUP	26	-0.0285		7470A	PPB		23 Dec 2019 11:56:55	U	SMPL			
K6355-01MS - 1	30604MS	15557	3.4491		7470A	PPB		23 Dec 2019 11:59:01	U	SMPL			
K6355-01MSD - 1	30604MSD	15594	3.4574		7470A	PPB		23 Dec 2019 12:01:07	U	SMPL			
K6363-01 - 1	T-2-CONTAINMENT-SUMP	188	0.0078		7470A	PPB		23 Dec 2019 12:03:13	U	SMPL			
K6363-02LX5 - 1		5	-0.0332		7470A	PPB		23 Dec 2019 12:05:20	U	SMPL			
K6117-09LX5 - 1		-1	-0.0345		7470A	PPB		23 Dec 2019 12:07:27	U	SMPL			
K6107-05LX5 - 1		10	-0.0321		7470A	PPB		23 Dec 2019 12:09:35	U	SMPL			
K6355-01LX5 - 1		-11	-0.0368		7470A	PPB		23 Dec 2019 12:11:43	U	SMPL			
PB125654TB - 1	PB125598TB	-16	-0.0379		7470A	PPB		23 Dec 2019 12:13:51	U	SMPL			
PB125655TB - 1	PB125629TB	-14	-0.0374		7470A	PPB		23 Dec 2019 12:15:55	U	SMPL			
CCV63 - 1	CCV63	23679	5.2677		7470A	PPB		23 Dec 2019 12:18:02	U	SMPL			
CCB63 - 1	CCB63	-21	-0.0390		7470A	PPB		23 Dec 2019 12:20:09	U	SMPL			
PB125656TB - 1	PB125596TB	12	-0.0316		7470A	PPB		23 Dec 2019 12:22:16	U	SMPL			
CCV64 - 1	CCV64	23169	5.1535		7470A	PPB		23 Dec 2019 12:24:23	U	SMPL			
CCB64 - 1	CCB64	-29	-0.0408		7470A	PPB		23 Dec 2019 12:26:30	U	SMPL			