

JC-2 300.0
 12-23-17 An

Clear table

ident	concentra tion F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-12-19_	12/19/19 15:26		AK/AP
STD2	0.2500	0.3990	0.3800	1.2380	0.3170	0.3550	2.0020	2019-12-19_	12/19/19 15:56		AK/AP
STD3	0.4400	0.6420	0.6580	2.2270	0.5560	0.9870	3.3430	2019-12-19_	12/19/19 16:25		AK/AP
STD4	0.8110	1.1640	1.1660	3.8820	0.9740	2.0690	5.8260	2019-12-19_	12/19/19 16:54		AK/AP
STD5	1.9030	2.8750	2.8740	9.5760	2.3840	5.1810	14.2170	2019-12-19_	12/19/19 17:23		AK/AP
STD6	3.8700	5.8950	5.9010	19.6930	4.9110	9.9480	29.3600	2019-12-19_	12/19/19 17:52		AK/AP
STD7	5.1270	7.6250	7.6200	25.3850	6.3580	12.4600	38.2530	2019-12-19_	12/19/19 18:21		AK/AP
ICV	2.0360	2.9970	2.9950	9.9910	2.4820	5.3130	14.8340	2019-12-19_	12/19/19 19:49		AK/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-12-19_	12/19/19 20:18		AK/AP
CCV	1.9410	2.9910	2.8470	9.8120	2.5020	4.6650	14.4270	2019-12-20_	12/20/19 9:49		AK/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-12-20_	12/20/19 10:19		AK/AP
LB106889BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-12-20_	12/20/19 11:17		AK/AP
LB106889BSW	1.9050	2.9860	2.9030	9.7880	2.4230	4.9630	14.3640	2019-12-20_	12/20/19 11:46		AK/AP
K6393-01	2.4680	374.9980	0.0000	11.7470	4.4520	0.0000	15.4850	2019-12-20_	12/20/19 15:32		AK/AP
K6393-02	0.2810	493.5270	0.0000	2.1170	1.2200	0.0000	73.9830	2019-12-20_	12/20/19 16:01		AK/AP
K6393-03	0.0000	284.0530	0.0000	2.6860	0.8660	0.0000	15.0950	2019-12-20_	12/20/19 16:30		AK/AP
K6393-04	0.0000	980.4690	0.0000	4.4150	1.6390	0.0000	148.4300	2019-12-20_	12/20/19 16:59		AK/AP
K6393-04DUP	0.0000	980.7830	0.0000	4.4070	1.6340	0.0000	148.5540	2019-12-20_	12/20/19 17:29		AK/AP
K6393-04MS	2.2730	929.0350	2.1910	13.8270	4.0000	9.5770	151.6980	2019-12-20_	12/20/19 17:58		AK/AP
K6393-04MSD	2.4470	927.5450	2.2450	14.1960	4.1300	10.0300	152.1650	2019-12-20_	12/20/19 18:27		AK/AP
CCV	1.9680	3.0510	2.9010	9.8910	2.5520	6.1470	14.3020	2019-12-20_	12/20/19 18:56		AK/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-12-20_	12/20/19 19:25		AK/AP


CALIBRATION OF COMPONENT F-

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.0755513 \cdot A + 1.93672$
 RSD: 5.227 %
 Correlation coefficient: 0.998845

IC2 CAL

12-19-19

AL

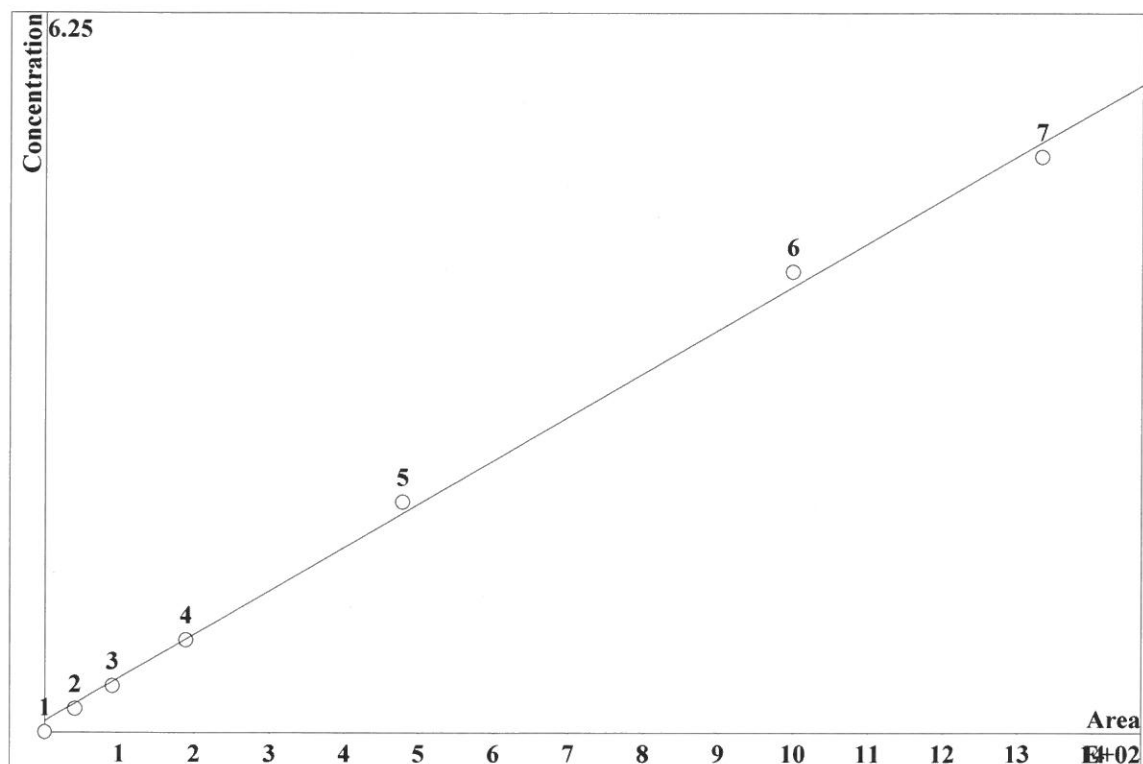

K3 = 0 K2 = 0 K1 = 0.0755513 K0 = 1.93672

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	1.602	40.47	0.2	20	5.516		
3	3.353	90.84	0.4	20	5.516		
4	7.546	189	0.8	20	5.516		
5	20.92	478.2	2	20	5.516		
6	45.31	998.7	4	20	5.516		
7	62.11	1332	5	20	5.516		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.140776 \cdot A + 1.87523$
 RSD: 3.786 %
 Correlation coefficient: 0.999394

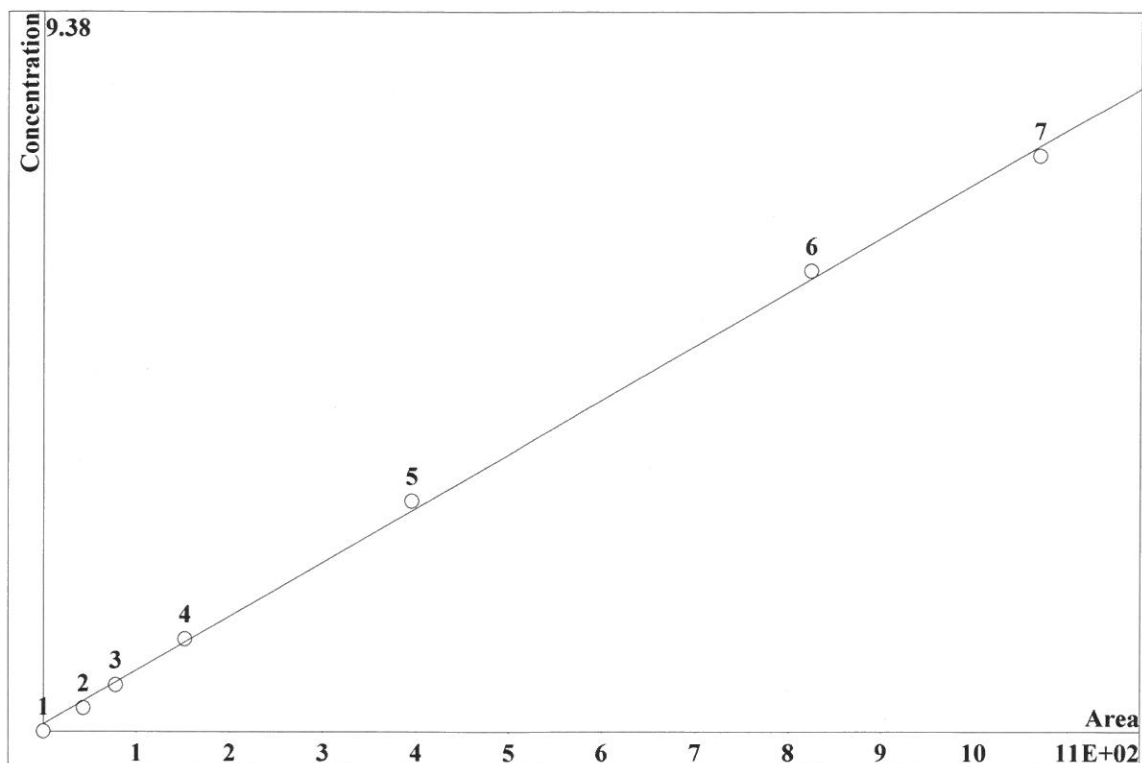

K3 = 0 K2 = 0 K1 = 0.140776 K0 = 1.87523

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.573	43.41	0.3	20	8.443		
3	5.183	77.84	0.6	20	8.443		
4	10.01	152	1.2	20	8.443		
5	26.33	395.2	3	20	8.443		
6	55.7	824.2	6	20	8.443		
7	72.45	1070	7.5	20	8.443		

ŷ

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.0627248 \cdot A + 2.30587$
 RSD: 3.646 %
 Correlation coefficient: 0.999438

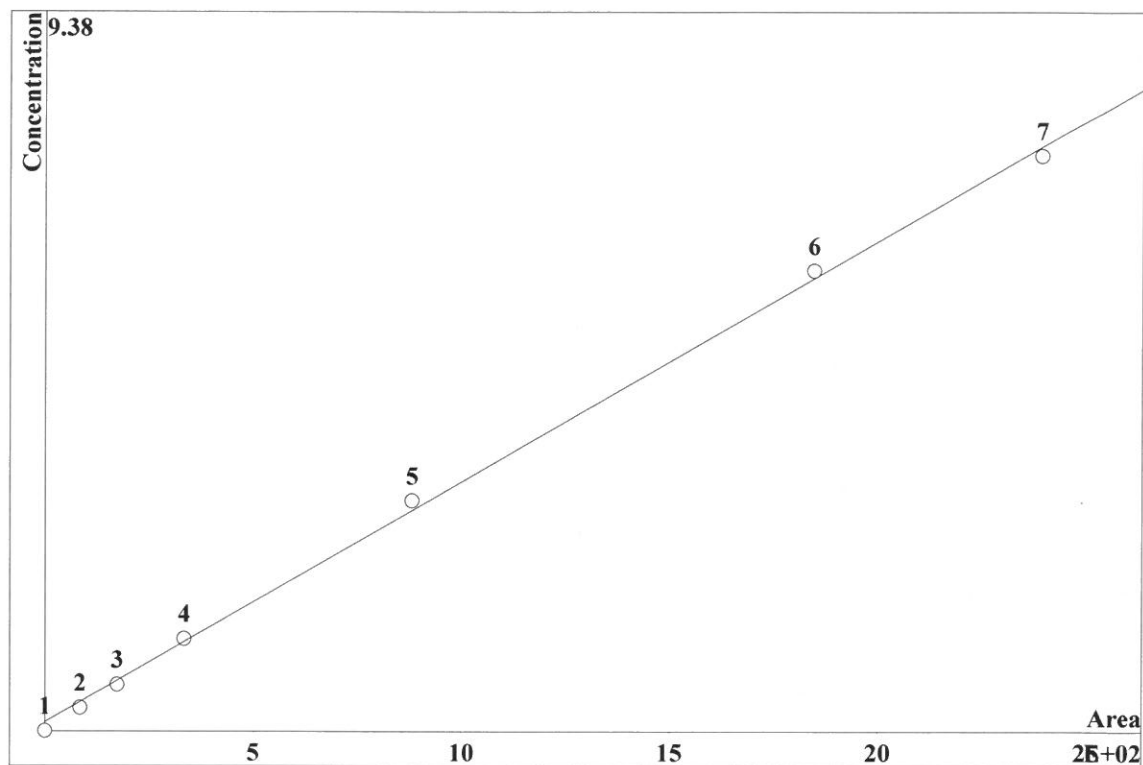

K3 = 0 K2 = 0 K1 = 0.0627248 K0 = 2.30587

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.615	84.53	0.3	20	10.18		
3	9.322	173.1	0.6	20	10.18		
4	17.96	334.9	1.2	20	10.18		
5	46.4	879.7	3	20	10.18		
6	93.12	1845	6	20	10.18		
7	120	2393	7.5	20	10.18		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.316728 \cdot A + 7.75699$
 RSD: 3.568 %
 Correlation coefficient: 0.999462

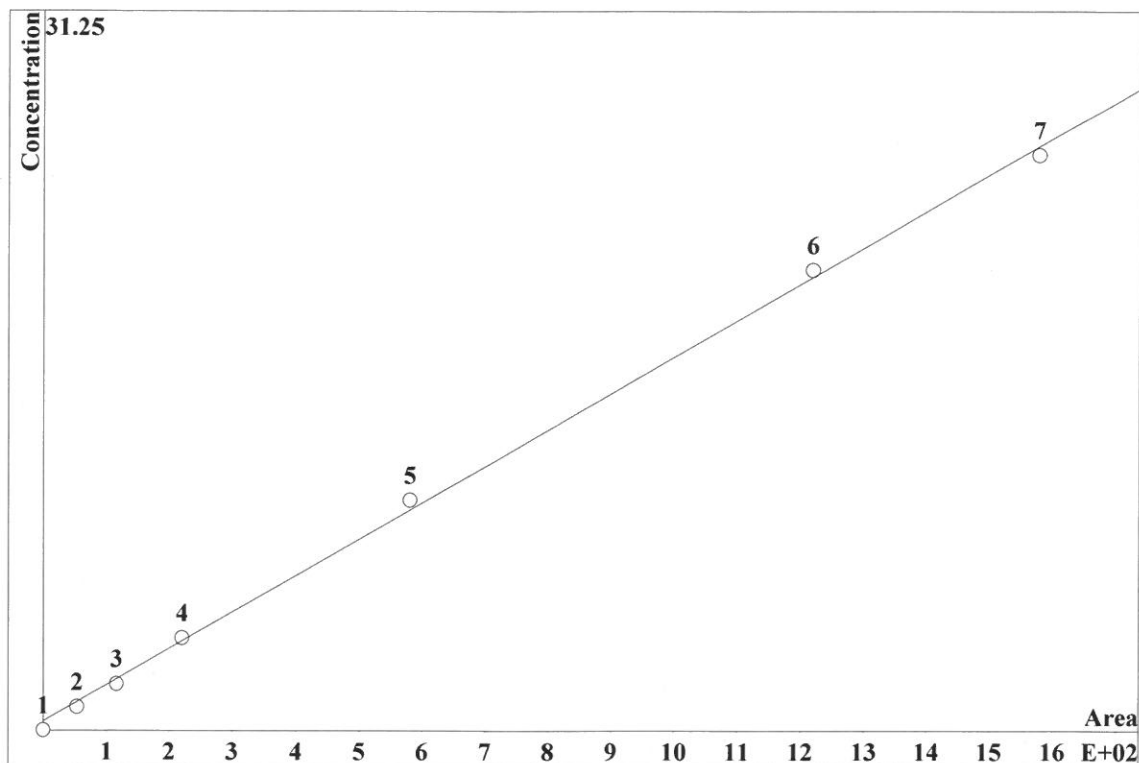

K3 = 0 K2 = 0 K1 = 0.316728 K0 = 7.75699

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.506	53.65	1	20	13.07		
3	5.233	116.1	2	20	13.07		
4	10.12	220.6	4	20	13.07		
5	26.95	580.2	10	20	13.07		
6	57.56	1219	20	20	13.07		
7	75.01	1578	25	20	13.07		

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.0567155 \cdot A + 1.9162$
 RSD: 3.923 %
 Correlation coefficient: 0.999349

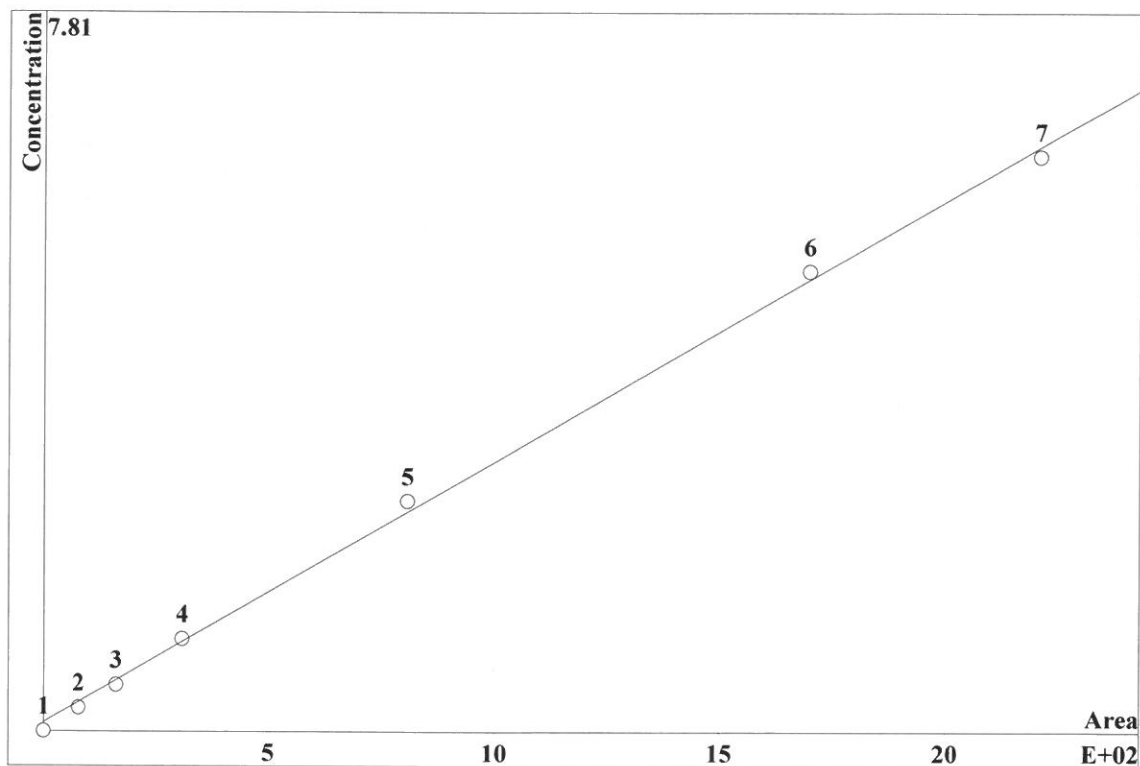

K3 = 0 K2 = 0 K1 = 0.0567155 K0 = 1.9162

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	3.046	77.91	0.25	20	15.04		
3	6.249	162.2	0.5	20	15.04		
4	11.98	309.8	1	20	15.04		
5	31.2	806.9	2.5	20	15.04		
6	65.71	1698	5	20	15.04		
7	85.55	2208	6.25	20	15.04		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.0942908 \cdot A - 3.46159$
 RSD: 2.433 %
 Correlation coefficient: 0.999750

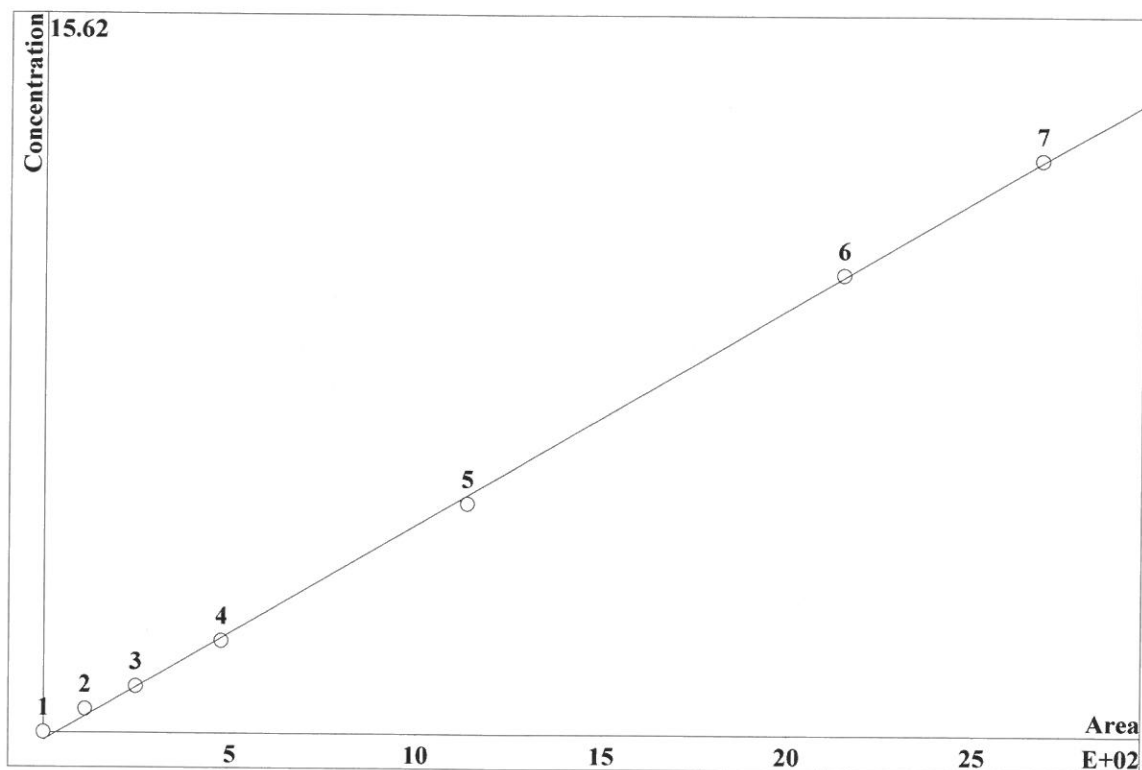

K3 = 0 K2 = 0 K1 = 0.0942908 K0 = -3.46159

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.415	112	0.5	20	20.37		
3	5.344	246	1	20	20.37		
4	10.51	475.5	2	20	20.37		
5	26.2	1136	5	20	20.37		
6	51.59	2147	10	20	20.37		
7	65.47	2680	12.5	20	20.37		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.181366 \cdot A + 12.4427$
 RSD: 4.550 %
 Correlation coefficient: 0.999125

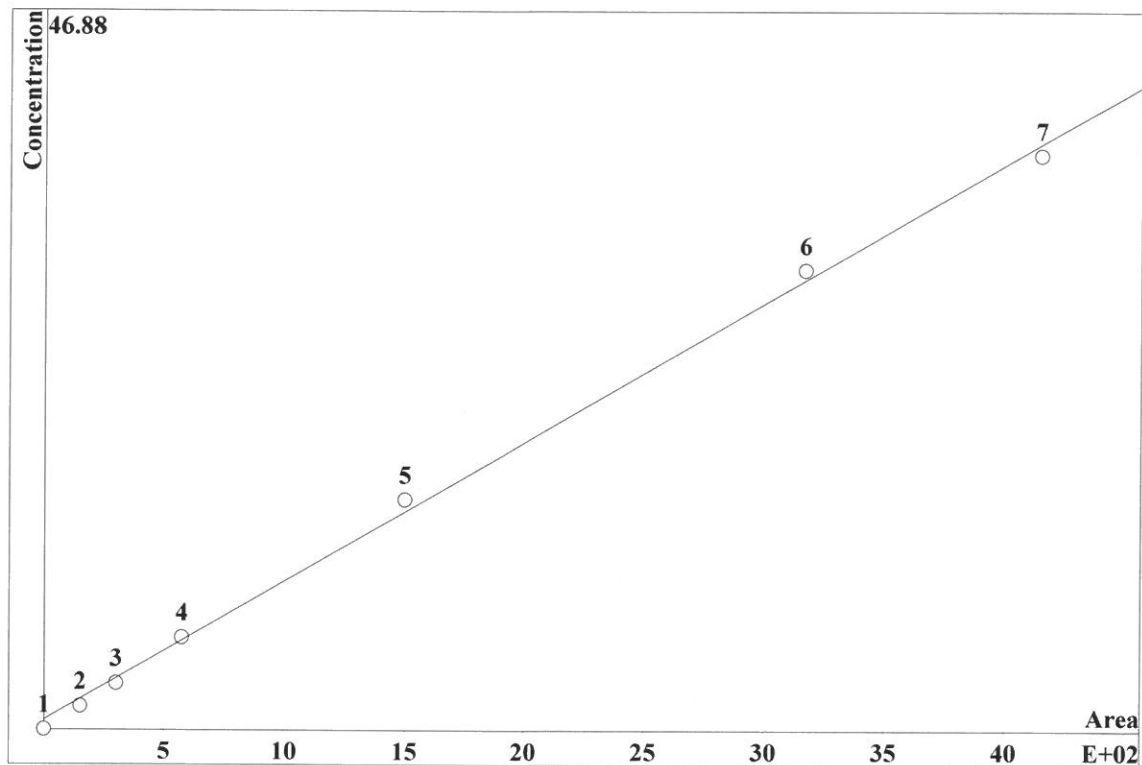

K3 = 0 K2 = 0 K1 = 0.181366 K0 = 12.4427

Base: Area

Ref.channel: chl

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	3.868	152.1	1.5	20	23.43		
3	7.718	300.1	3	20	23.43		
4	14.7	573.8	6	20	23.43		
5	38.7	1499	15	20	23.43		
6	82.78	3169	30	20	23.43		
7	108.7	4150	37.5	20	23.43		

Report date: 12/23/2019 11:14:07 AM
Printed by: wet


Ident: STD1
Analysis from: 12/19/2019 3:26:59 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:00 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24042

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

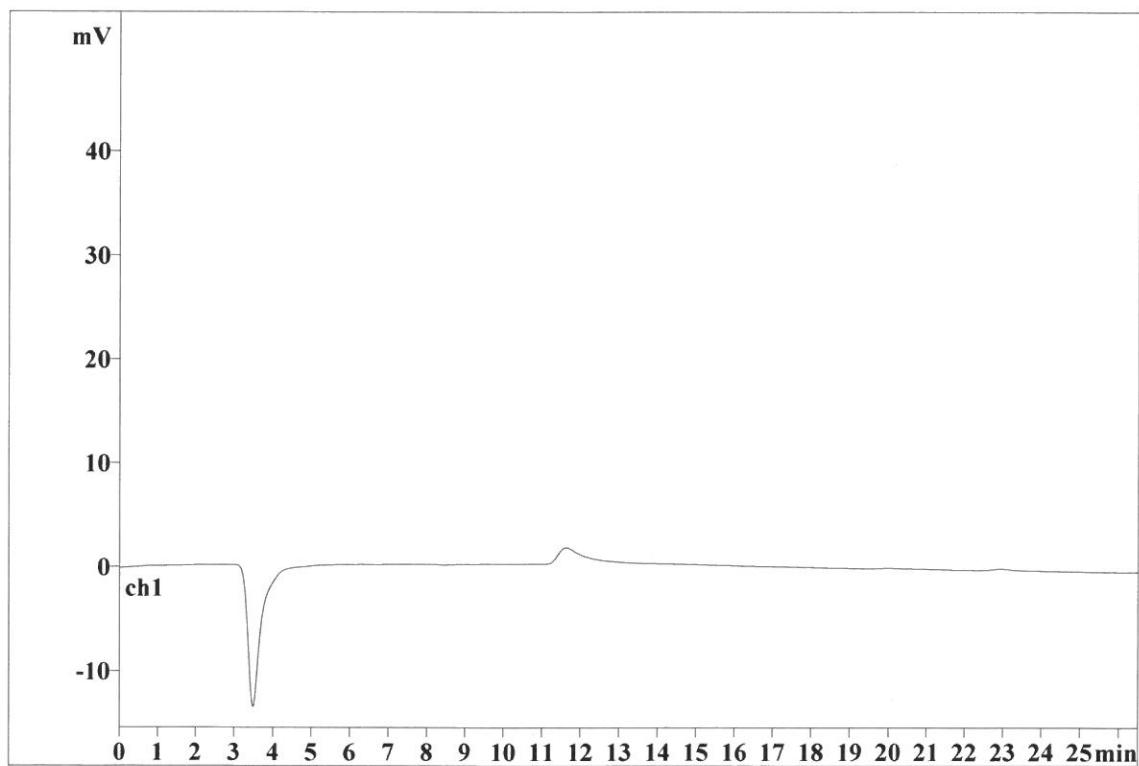

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:14:24 AM
Printed by: wet


Ident: STD2
Analysis from: 12/19/2019 3:56:07 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:00 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24043

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

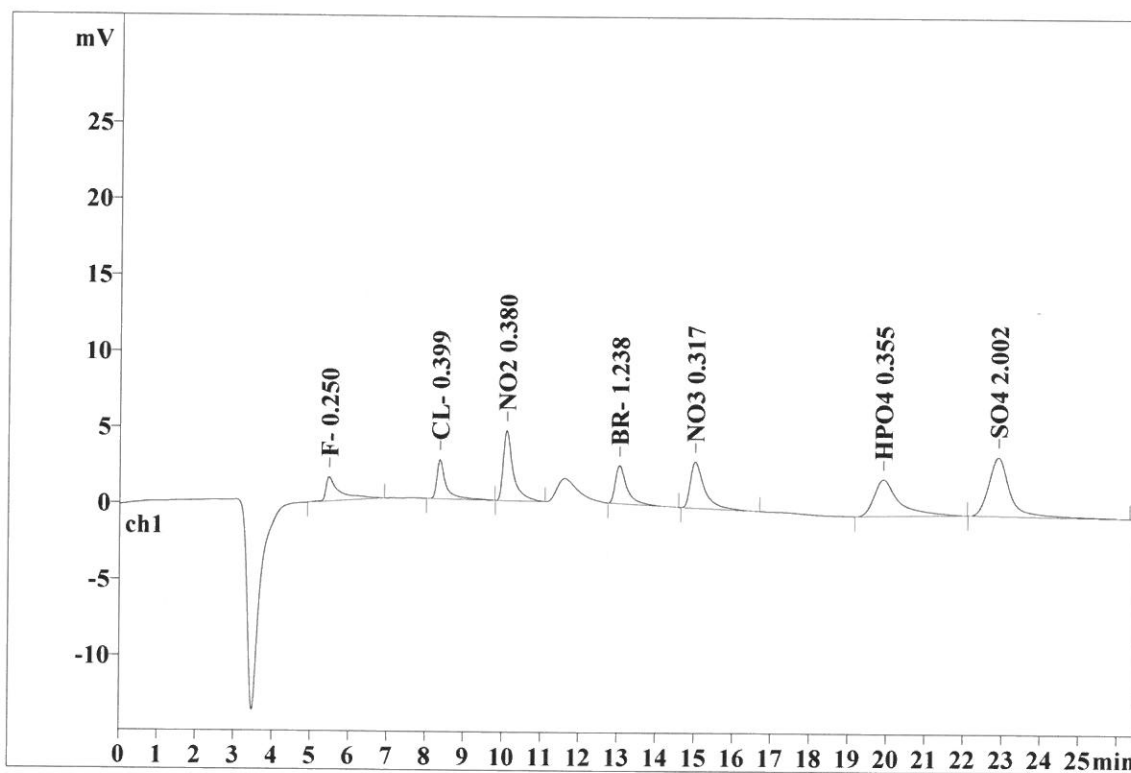

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.46	0.274	1.60	7.76	40.468	7.17
2	8.35	0.206	2.57	12.46	43.408	7.69
3	10.08	0.245	4.61	22.37	84.529	14.98
4	13.03	0.294	2.51	12.15	53.654	9.51
5	15.00	0.350	3.04	14.76	77.906	13.81
6	19.89	0.594	2.41	11.70	112.029	19.86
7	22.87	0.536	3.87	18.75	152.123	26.97
7	26.50	0.357	20.62	99.96	564.118	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:14:38 AM
Printed by: wet


Ident: STD3
Analysis from: 12/19/2019 4:25:15 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:01 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24044

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

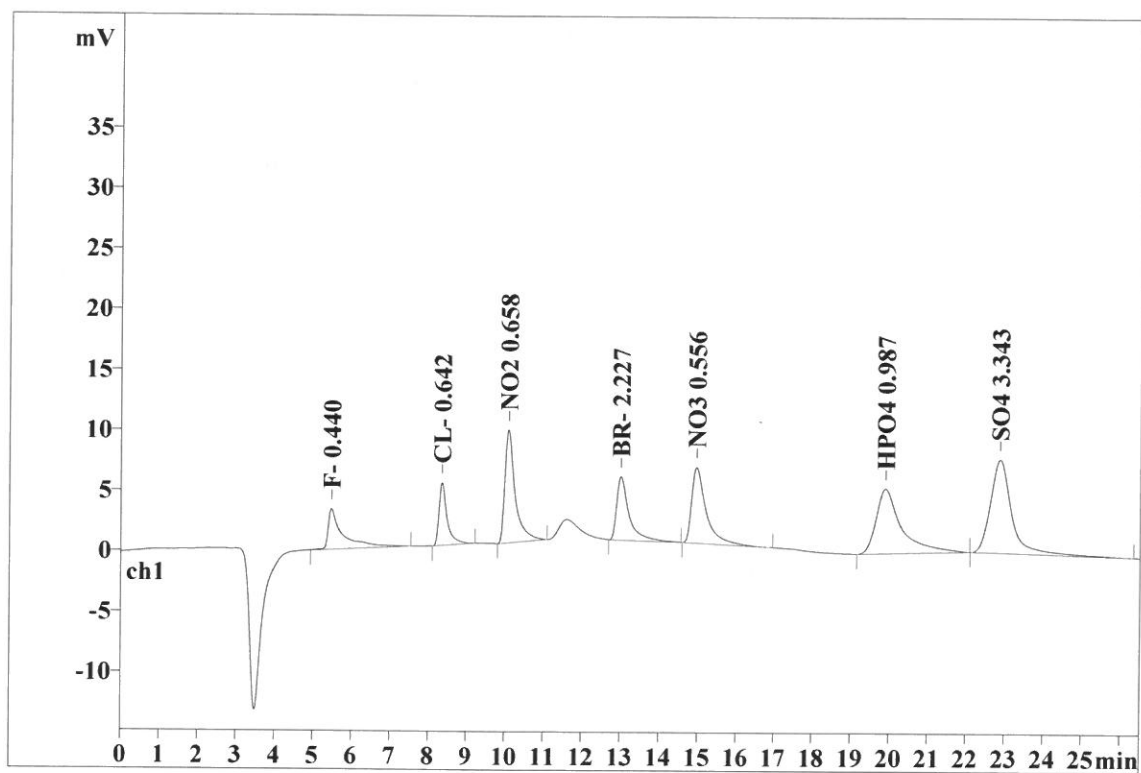

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.46	0.273	3.35	7.90	90.838	7.79
2	8.34	0.204	5.18	12.22	77.838	6.67
3	10.08	0.250	9.32	21.98	173.143	14.85
4	13.00	0.295	5.23	12.34	116.126	9.96
5	14.96	0.350	6.25	14.74	162.230	13.91
6	19.90	0.588	5.34	12.60	246.023	21.09
7	22.88	0.533	7.72	18.20	300.076	25.73
7	26.50	0.356	42.40	99.99	1166.274	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:14:51 AM
Printed by: wet


Ident: STD4
Analysis from: 12/19/2019 4:54:22 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:01 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24045

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

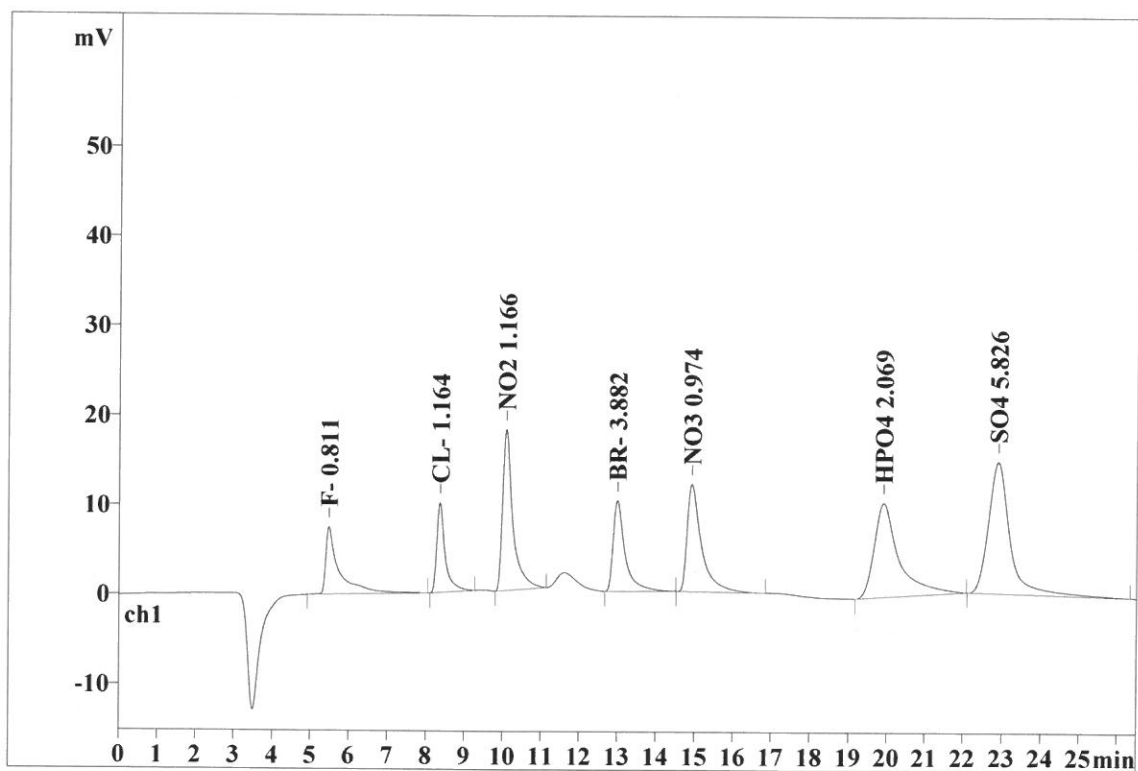

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.47	0.258	7.54	9.11	188.985	8.38
2	8.35	0.204	10.01	12.09	151.994	6.74
3	10.07	0.248	17.96	21.68	334.935	14.85
4	12.98	0.292	10.12	12.22	220.644	9.78
5	14.91	0.350	11.98	14.46	309.778	13.73
6	19.90	0.579	10.50	12.68	475.545	21.08
7	22.89	0.531	14.70	17.75	573.814	25.44
7	26.50	0.352	82.82	99.99	2255.695	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:15:01 AM
Printed by: wet


Ident: STD5
Analysis from: 12/19/2019 5:23:31 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:01 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24046

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

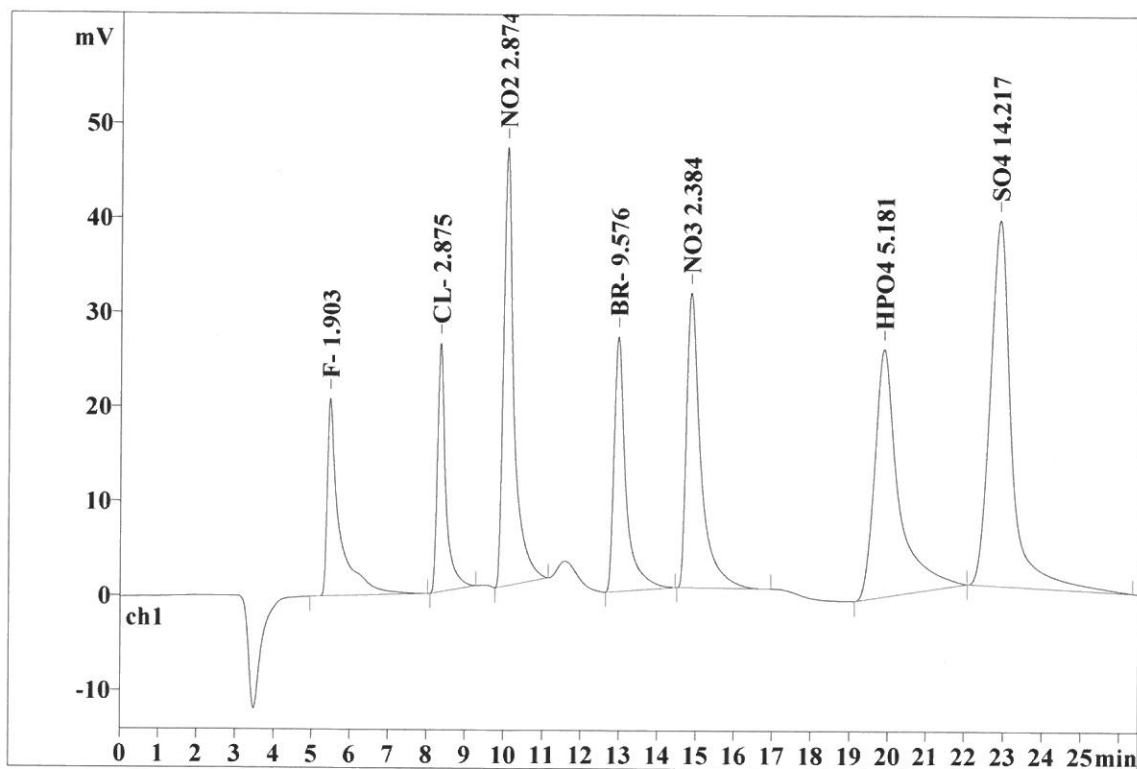

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.47	0.243	20.92	9.65	478.173	8.28
2	8.34	0.200	26.32	12.15	395.195	6.84
3	10.04	0.253	46.40	21.41	879.705	15.23
4	12.95	0.286	26.95	12.44	580.168	10.05
5	14.84	0.350	31.19	14.40	806.924	13.97
6	19.87	0.555	26.20	12.09	1135.752	19.67
7	22.87	0.524	38.70	17.86	1499.142	25.96
7	26.50	0.345	216.68	100.00	5775.059	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:15:11 AM
Printed by: wet


Ident: STD6
Analysis from: 12/19/2019 5:52:39 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:01 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24047

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

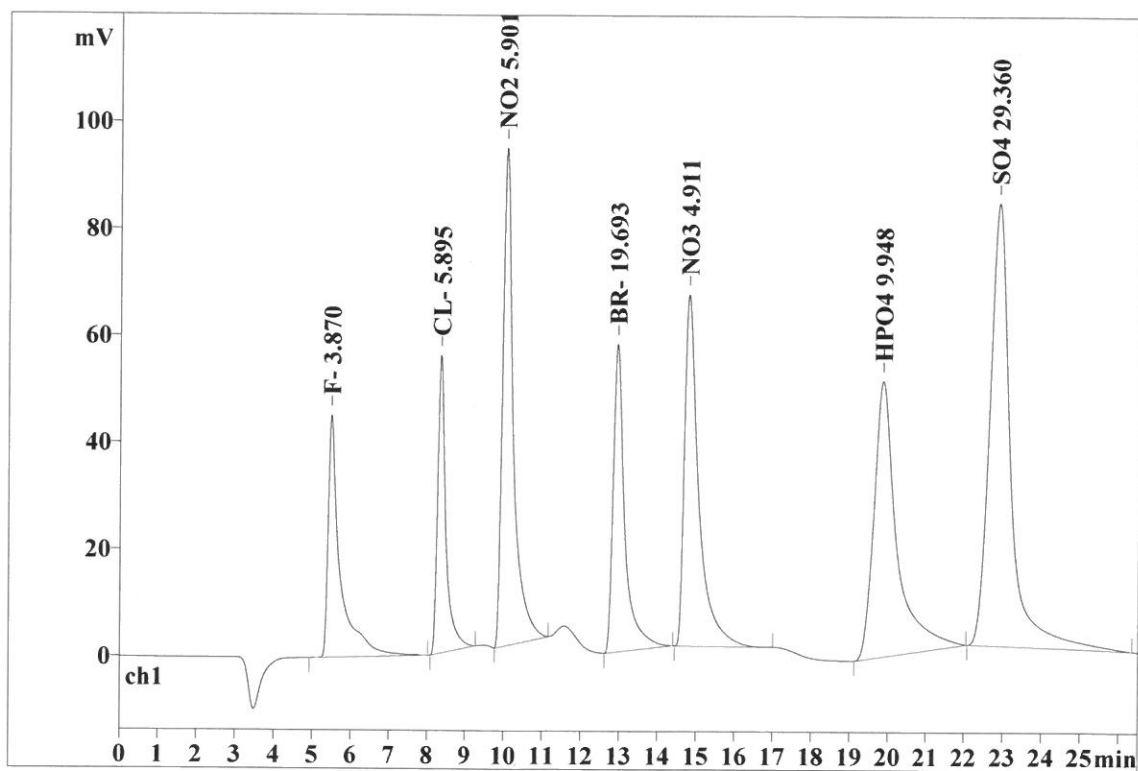

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.48	0.240	45.31	10.03	998.717	8.39
2	8.34	0.198	55.70	12.33	824.179	6.93
3	10.03	0.269	93.12	20.61	1844.817	15.50
4	12.93	0.281	57.56	12.74	1219.057	10.24
5	14.79	0.350	65.71	14.55	1698.186	14.27
6	19.85	0.535	51.59	11.42	2146.735	18.04
7	22.87	0.515	82.77	18.32	3169.042	26.63
7	26.50	0.341	451.76	100.00	11900.734	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:15:25 AM
Printed by: wet


Ident: STD7
Analysis from: 12/19/2019 6:21:47 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:59 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24048

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

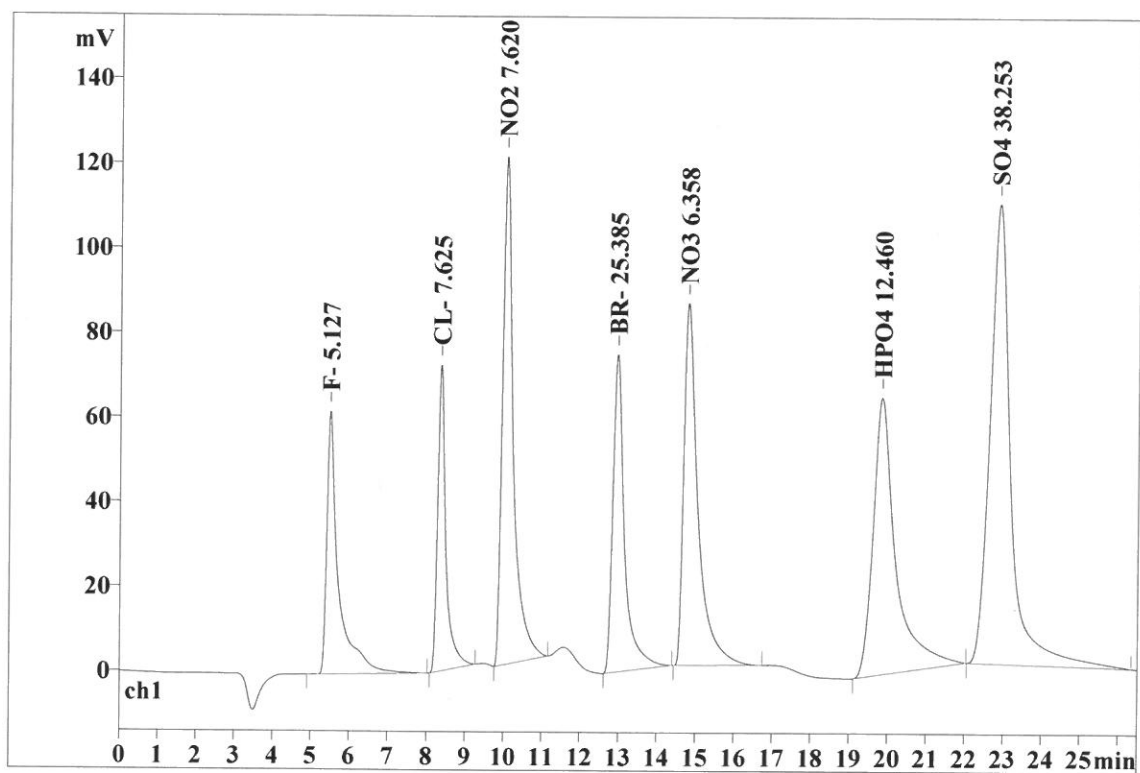

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.49	0.240	62.11	10.54	1331.550	8.64
2	8.34	0.198	72.44	12.29	1069.966	6.94
3	10.02	0.270	120.03	20.37	2392.969	15.53
4	12.94	0.280	75.01	12.73	1578.430	10.24
5	14.78	0.350	85.55	14.52	2208.140	14.33
6	19.83	0.528	65.47	11.11	2679.590	17.39
7	22.86	0.513	108.66	18.44	4149.674	26.93
7	26.50	0.340	589.27	100.00	15410.320	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:16:05 AM
Printed by: wet


Ident: ICV
Analysis from: 12/19/2019 7:49:10 PM
File: _2019-12-19_

Last save: 12/20/2019 9:10:00 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24051

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

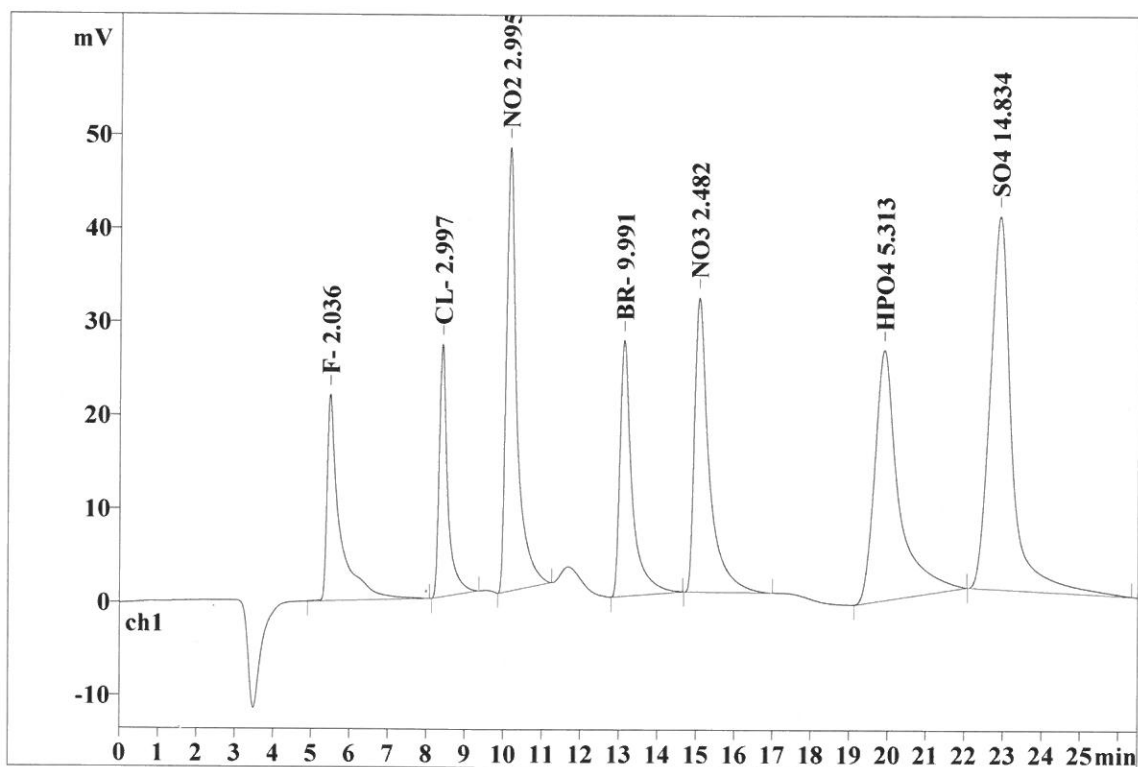

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.48	0.251	22.06	9.93	513.278	8.52
2	8.39	0.204	27.02	12.17	412.466	6.85
3	10.13	0.258	47.48	21.38	918.295	15.25
4	13.11	0.294	27.35	12.32	606.385	10.07
5	15.05	0.362	31.45	14.16	841.437	13.97
6	19.88	0.560	26.76	12.05	1163.557	19.32
7	22.88	0.531	39.94	17.99	1567.230	26.02
7	26.50	0.351	222.06	100.00	6022.648	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:16:16 AM
Printed by: wet


Ident: ICB
Analysis from: 12/19/2019 8:18:19 PM
File: _2019-12-19_

Last save: 12/20/2019 9:10:00 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24052

Last save: 12/19/2019 6:19

SAMPLE:
:
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

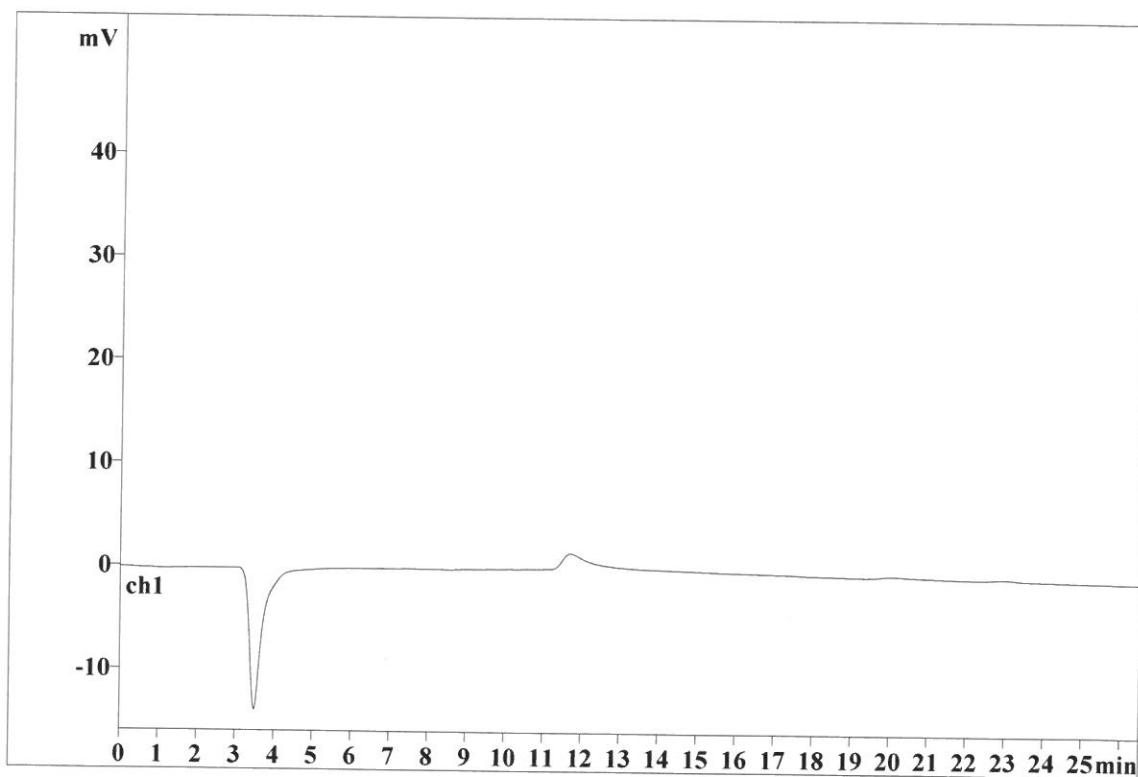

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:18:32 AM
Printed by: wet


Ident: CCV
Analysis from: 12/20/2019 9:49:36 AM
File: _2019-12-20_

Last save: 12/20/2019 11:53:32 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24055

Last save: 12/20/2019 9:09

SAMPLE:
: CT/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

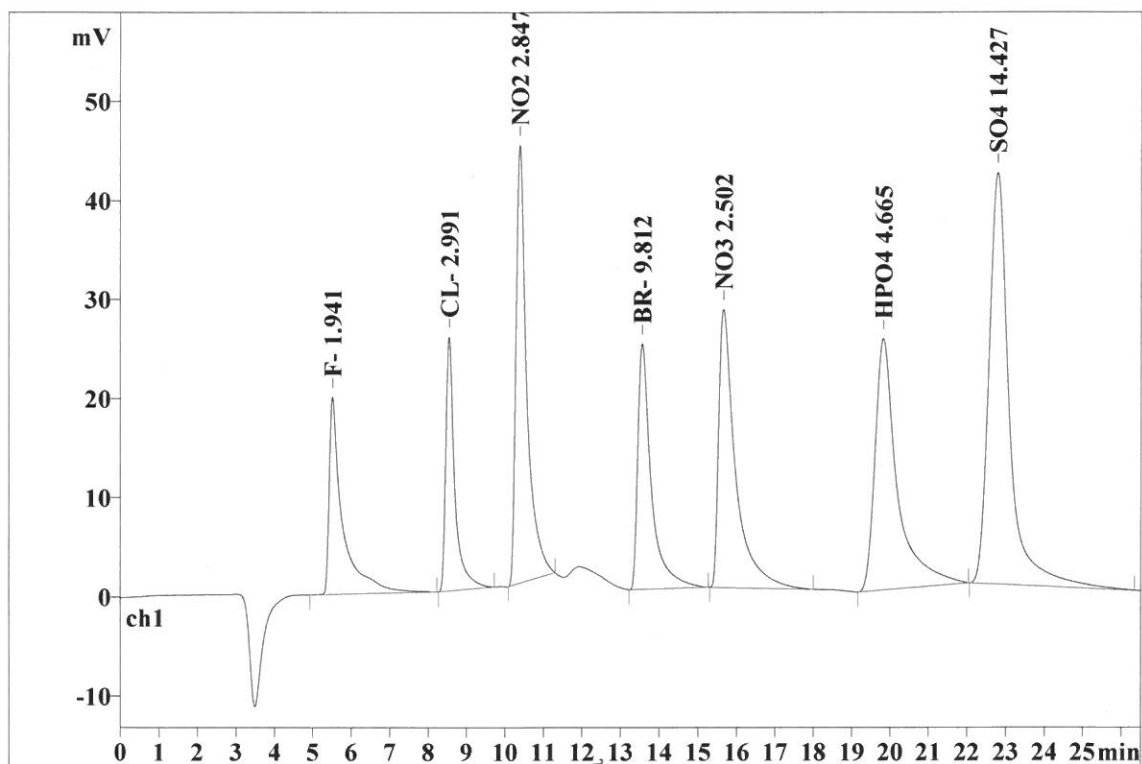

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.51	0.268	19.88	9.49	488.145	8.47
2	8.54	0.211	25.60	12.22	411.666	7.14
3	10.37	0.269	44.24	21.12	870.879	15.11
4	13.56	0.317	24.76	11.82	595.106	10.33
5	15.65	0.399	28.06	13.40	848.621	14.73
6	19.82	0.526	25.34	12.10	1026.126	17.81
7	22.79	0.501	41.54	19.83	1522.277	26.42
7	26.50	0.356	209.42	100.00	5762.820	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:18:41 AM
Printed by: wet


Ident: CCB
Analysis from: 12/20/2019 10:19:09 AM
File: _2019-12-20_

Last save: 12/20/2019 10:45:39 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24056

Last save: 12/20/2019 9:09

SAMPLE:
: CT/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

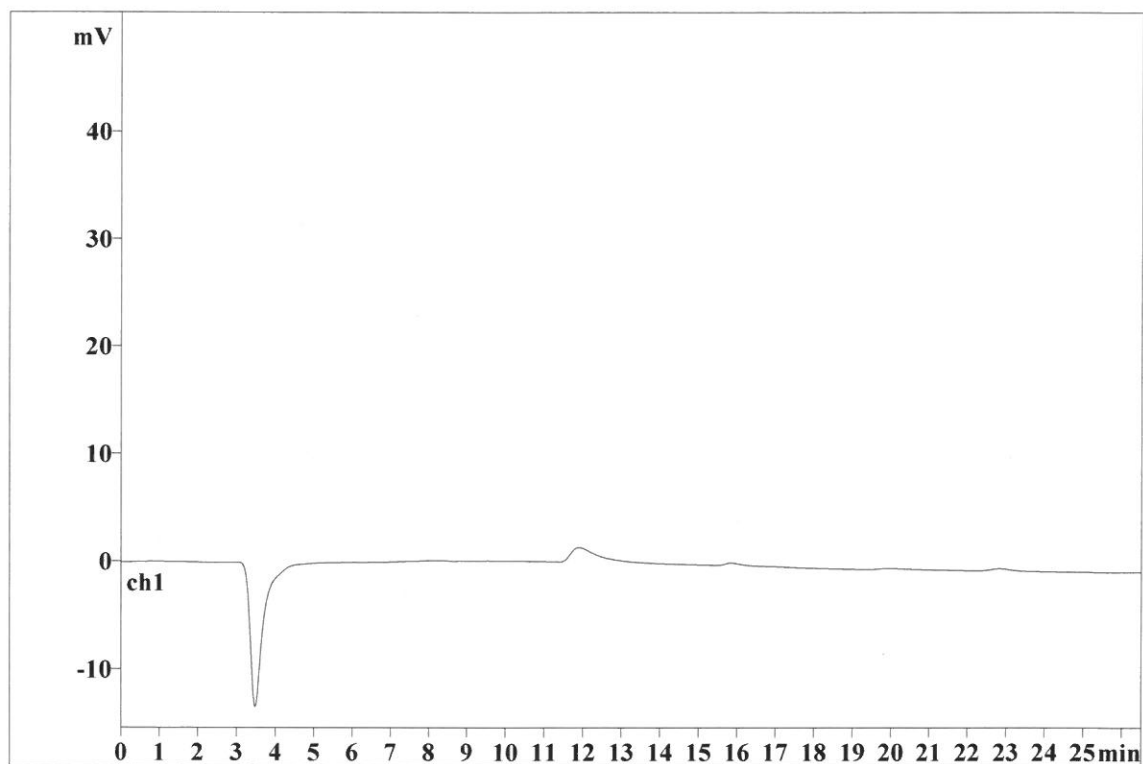

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:18:51 AM
Printed by: wet


Ident: LB106889BLW
Analysis from: 12/20/2019 11:17:32 AM
File: _2019-12-20_

Last save: 12/23/2019 11:13:54 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24058

Last save: 12/20/2019 9:09

SAMPLE:
: CT/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

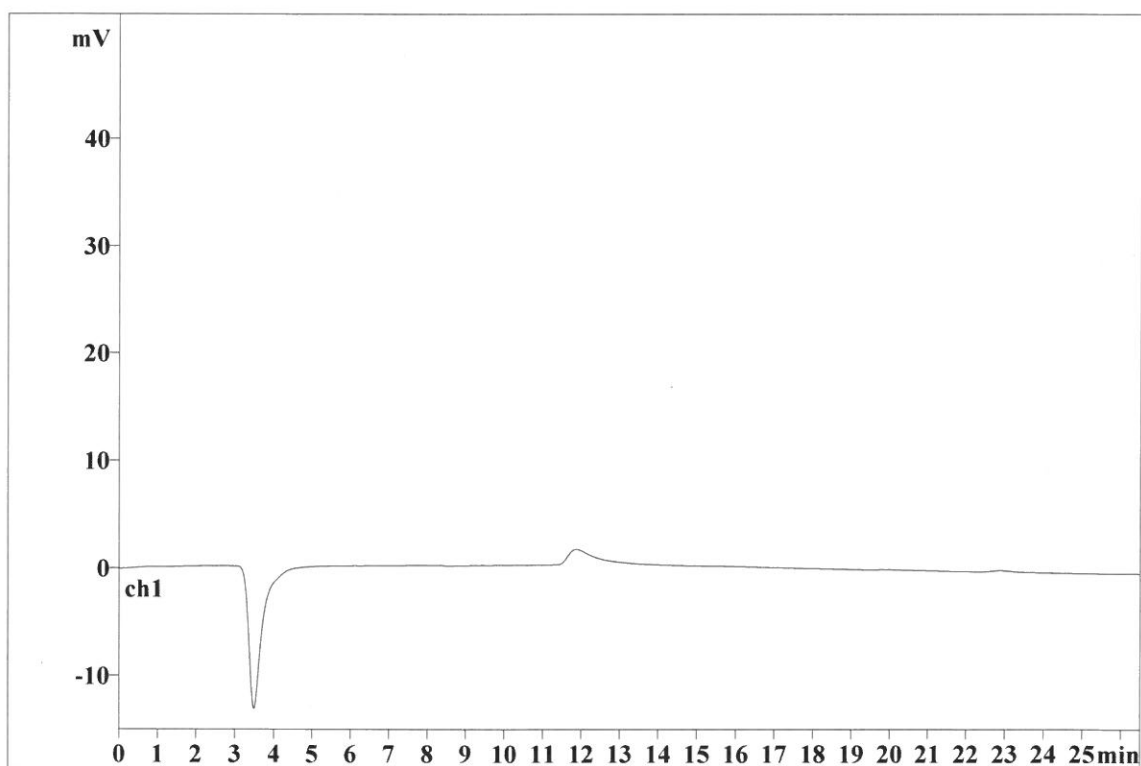

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:19:10 AM
Printed by: wet


Ident: LB106889BSW
Analysis from: 12/20/2019 11:46:41 AM
File: _2019-12-20_

Last save: 12/23/2019 11:13:54 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24059

Last save: 12/20/2019 9:09

SAMPLE:
: CT/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

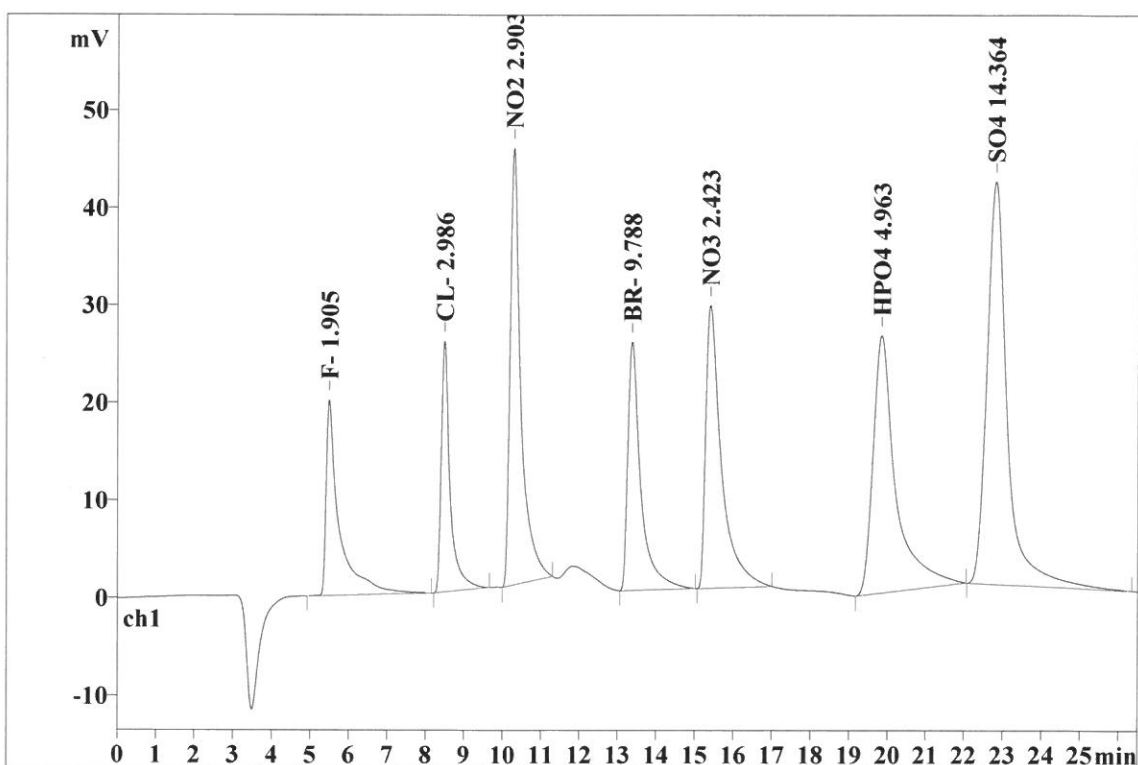

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.49	0.255	20.08	9.43	478.684	8.26
2	8.48	0.209	25.73	12.09	410.849	7.09
3	10.27	0.266	44.83	21.06	888.926	15.33
4	13.37	0.307	25.49	11.98	593.599	10.24
5	15.40	0.383	28.99	13.62	820.486	14.15
6	19.83	0.532	26.41	12.41	1089.365	18.79
7	22.81	0.502	41.31	19.41	1515.414	26.14
7	26.50	0.351	212.85	100.00	5797.324	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:29:29 AM
Printed by: wet


Ident: K6893-01
Analysis from: 12/20/2019 3:32:18 PM
File: _2019-12-20_

Last save: 12/23/2019 11:29:26 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24062

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

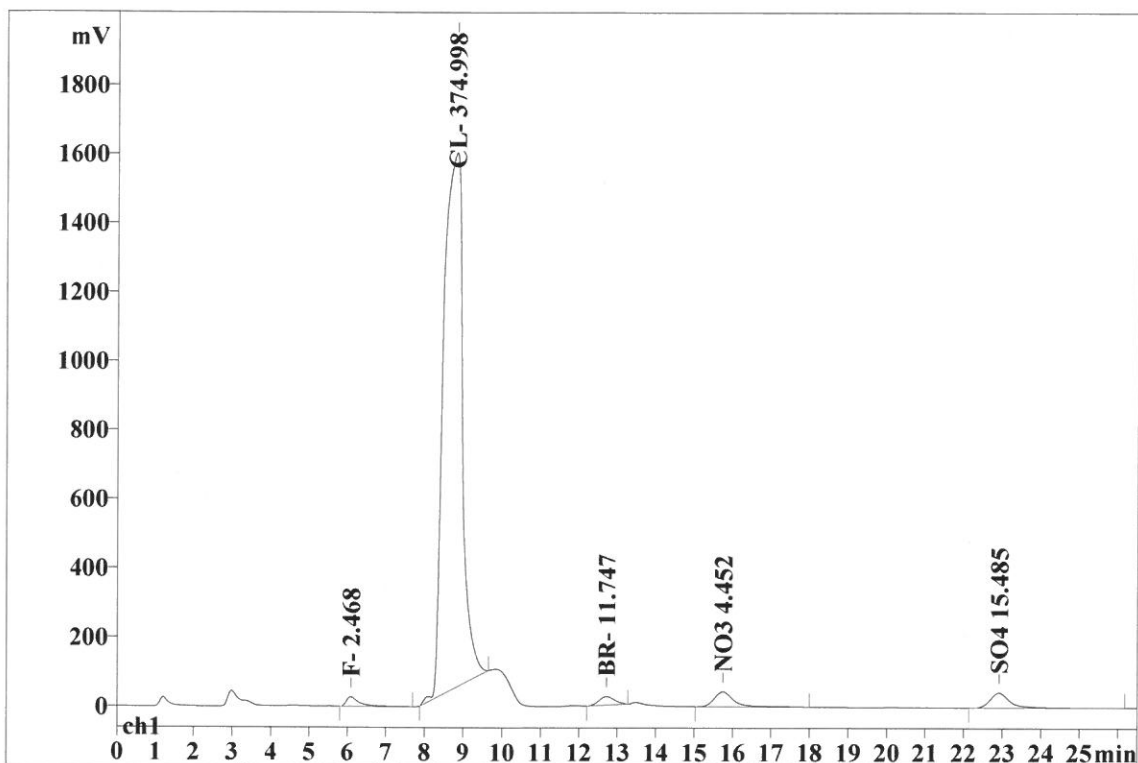

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.08	0.308	27.11	1.61	627.809	1.09
2	8.79	0.536	1549.74	91.77	53262.743	92.18
3	0.00	0.000	0.00	0.00	0.000	0.00
4	12.71	0.459	24.93	1.48	717.262	1.24
5	15.75	0.492	43.10	2.55	1536.022	2.66
6	0.00	0.000	0.00	0.00	0.000	0.00
7	22.92	0.506	43.77	2.59	1639.005	2.84
7	26.50	0.329	1688.63	100.00	57782.841	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:30:19 AM
Printed by: wet


Ident: K6893-02
Analysis from: 12/20/2019 4:01:28 PM
File: _2019-12-20_

Last save: 12/23/2019 11:30:15 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24063

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

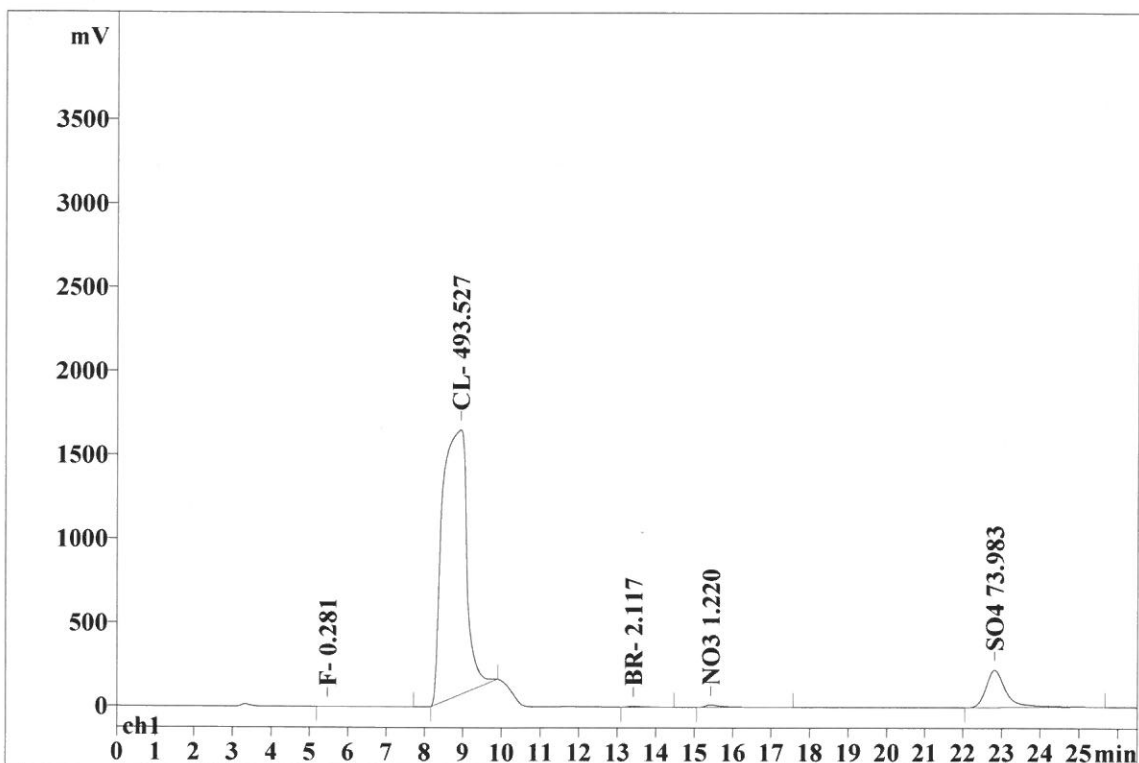

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.46	0.342	1.65	0.09	48.747	0.06
2	8.91	0.709	1579.81	86.65	70102.210	89.02
3	0.00	0.000	0.00	0.00	0.000	0.00
4	13.42	0.306	4.94	0.27	109.175	0.14
5	15.42	0.377	13.81	0.76	396.325	0.50
6	0.00	0.000	0.00	0.00	0.000	0.00
7	22.82	0.494	222.97	12.23	8089.855	10.27
7	26.50	0.318	1823.18	100.00	78746.312	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:32:31 AM
Printed by: wet


Ident: K6093-03
Analysis from: 12/20/2019 4:30:37 PM
File: _2019-12-20_

Last save: 12/23/2019 11:32:25 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24064

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

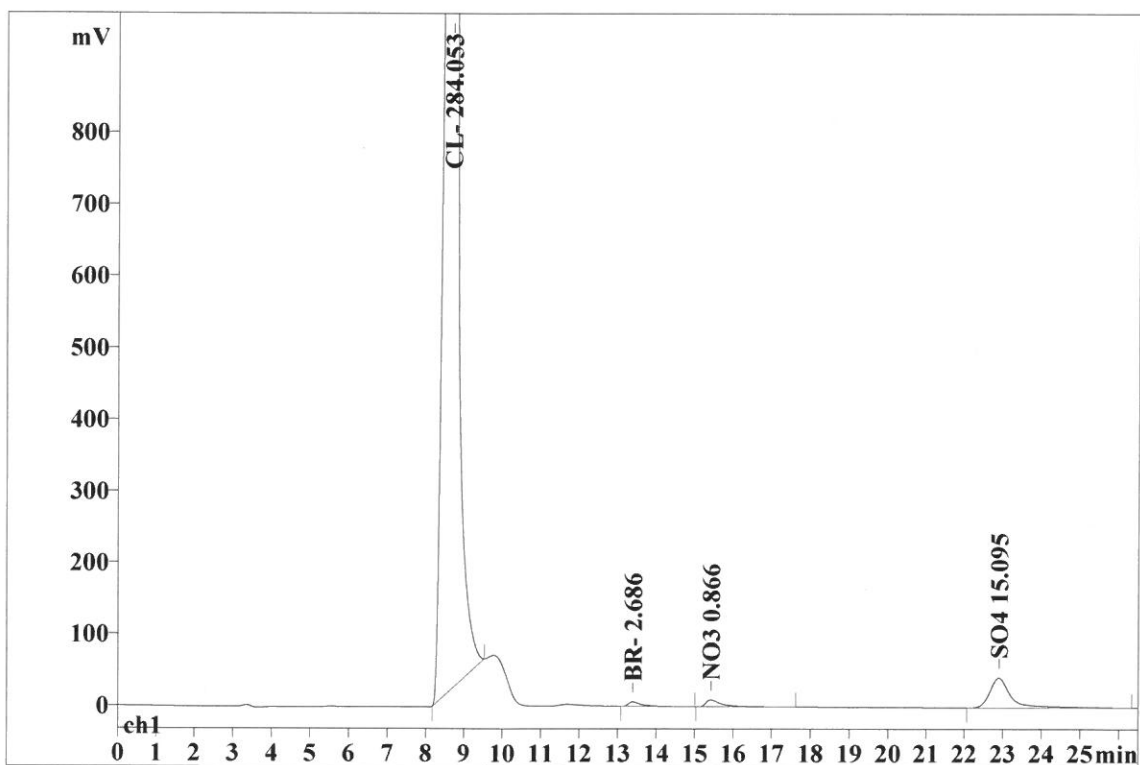

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.67	0.404	1521.38	96.36	40342.192	95.25
3	0.00	0.000	0.00	0.00	0.000	0.00
4	13.39	0.306	6.23	0.39	145.126	0.34
5	15.42	0.374	9.60	0.61	271.765	0.64
6	0.00	0.000	0.00	0.00	0.000	0.00
7	22.90	0.513	41.55	2.63	1595.992	3.77
7	26.50	0.228	1578.76	99.99	42355.075	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:32:57 AM
Printed by: wet


Ident: K6093-04
Analysis from: 12/20/2019 4:59:46 PM
File: 2019-12-20

Last save: 12/23/2019 11:32:52 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24065

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

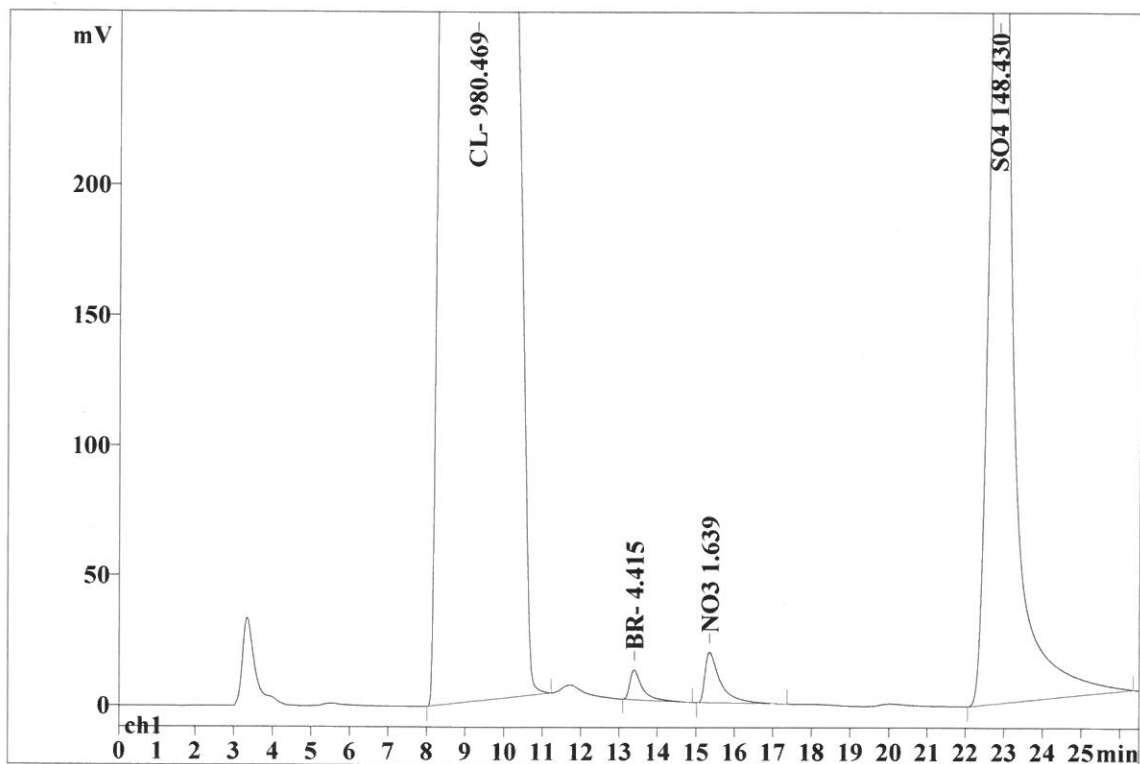

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.25	1.220	1701.64	78.50	139282.024	89.07
3	0.00	0.000	0.00	0.00	0.000	0.00
4	13.39	0.298	11.37	0.52	254.276	0.16
5	15.36	0.373	19.40	0.90	544.355	0.35
6	0.00	0.000	0.00	0.00	0.000	0.00
7	22.80	0.505	435.25	20.08	16299.436	10.42
7	26.50	0.342	2167.66	100.00	156380.089	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:33:20 AM
Printed by: wet


Ident: K6993-04DUP
Analysis from: 12/20/2019 5:29:01 PM
File: _2019-12-20_

Last save: 12/23/2019 11:33:19 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24066

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

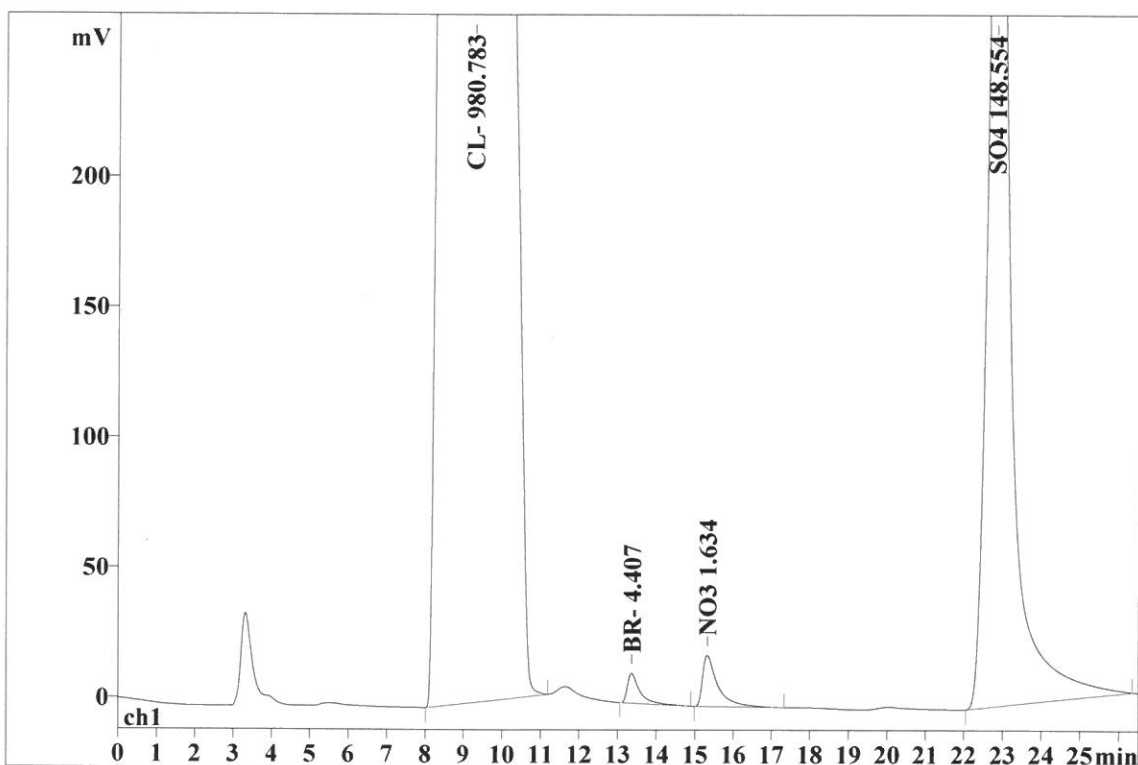

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.24	1.222	1700.49	78.48	139326.752	89.06
3	0.00	0.000	0.00	0.00	0.000	0.00
4	13.36	0.295	11.48	0.53	253.795	0.16
5	15.32	0.368	19.59	0.90	542.590	0.35
6	0.00	0.000	0.00	0.00	0.000	0.00
7	22.80	0.505	435.36	20.09	16313.079	10.43
7	26.50	0.341	2166.91	100.00	156436.217	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:37:46 AM
Printed by: wet

Ident: K6093-04MS
Analysis from: 12/20/2019 5:58:10 PM
File: _2019-12-20_


Last save: 12/23/2019 11:37:45 AM

Manual peaks!

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24067

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

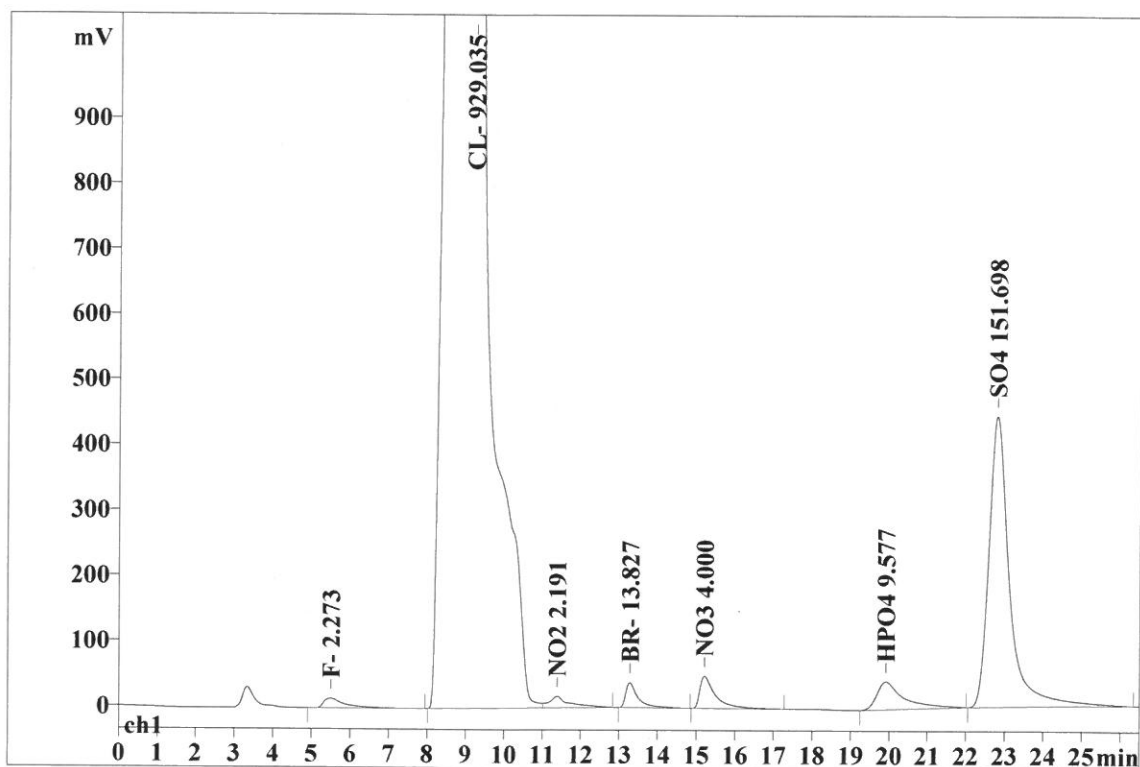

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.50	0.510	14.86	0.64	576.112	0.37
2	9.18	1.141	1696.82	73.67	131974.815	85.61
3	11.39	0.391	17.52	0.76	661.892	0.43
4	13.29	0.290	38.19	1.66	848.614	0.55
5	15.21	0.372	49.07	2.13	1376.637	0.89
6	19.91	0.622	42.44	1.84	2068.118	1.34
7	22.79	0.508	444.45	19.30	16659.758	10.81
7	26.50	0.548	2303.35	100.00	154165.947	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:39:16 AM
Printed by: wet

Ident: K6893-04MSD
Analysis from: 12/20/2019 6:27:20 PM
File: _2019-12-20_


Last save: 12/23/2019 11:39:15 AM

Manual peaks!

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24068

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

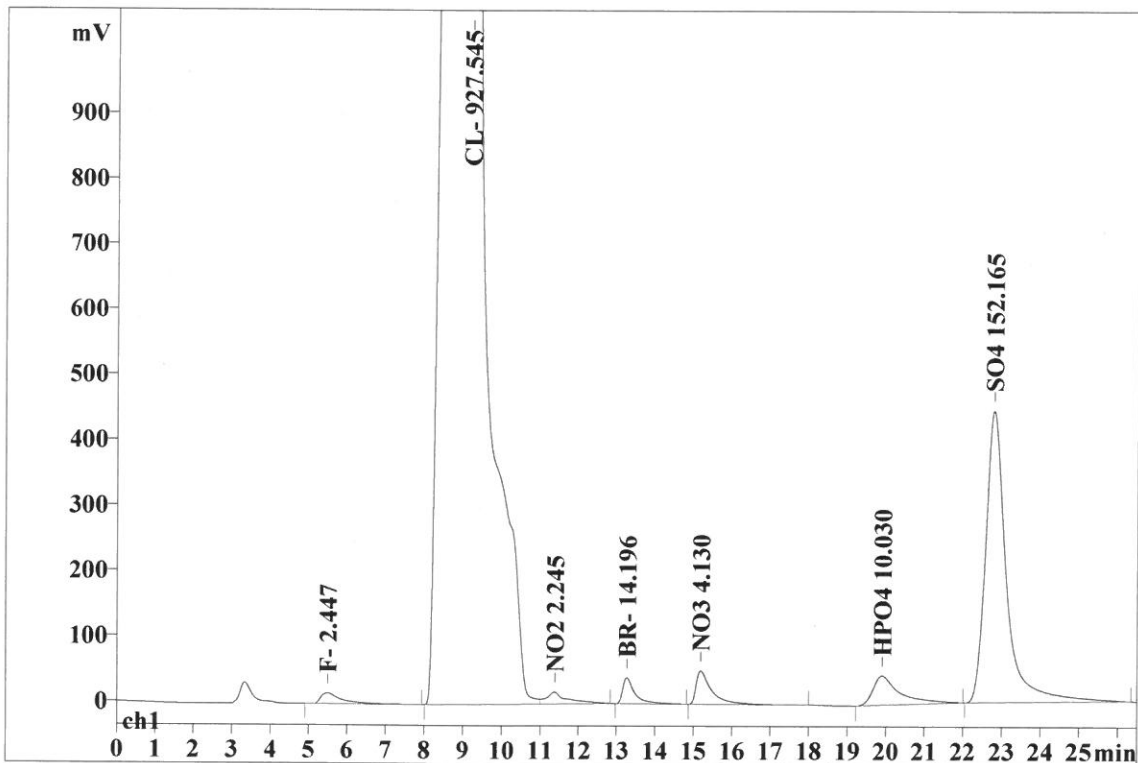

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.50	0.504	16.36	0.71	622.197	0.40
2	9.17	1.140	1695.64	73.40	131763.123	85.43
3	11.37	0.392	17.95	0.78	678.978	0.44
4	13.27	0.288	39.51	1.71	871.916	0.57
5	15.19	0.371	50.75	2.20	1422.621	0.92
6	19.90	0.618	44.61	1.93	2164.162	1.40
7	22.78	0.508	445.27	19.28	16711.269	10.83
7	26.50	0.546	2310.09	100.00	154234.266	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:39:49 AM
Printed by: wet


Ident: CCV
Analysis from: 12/20/2019 6:56:32 PM
File: _2019-12-20_

Last save: 12/20/2019 7:23:03 PM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24069

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

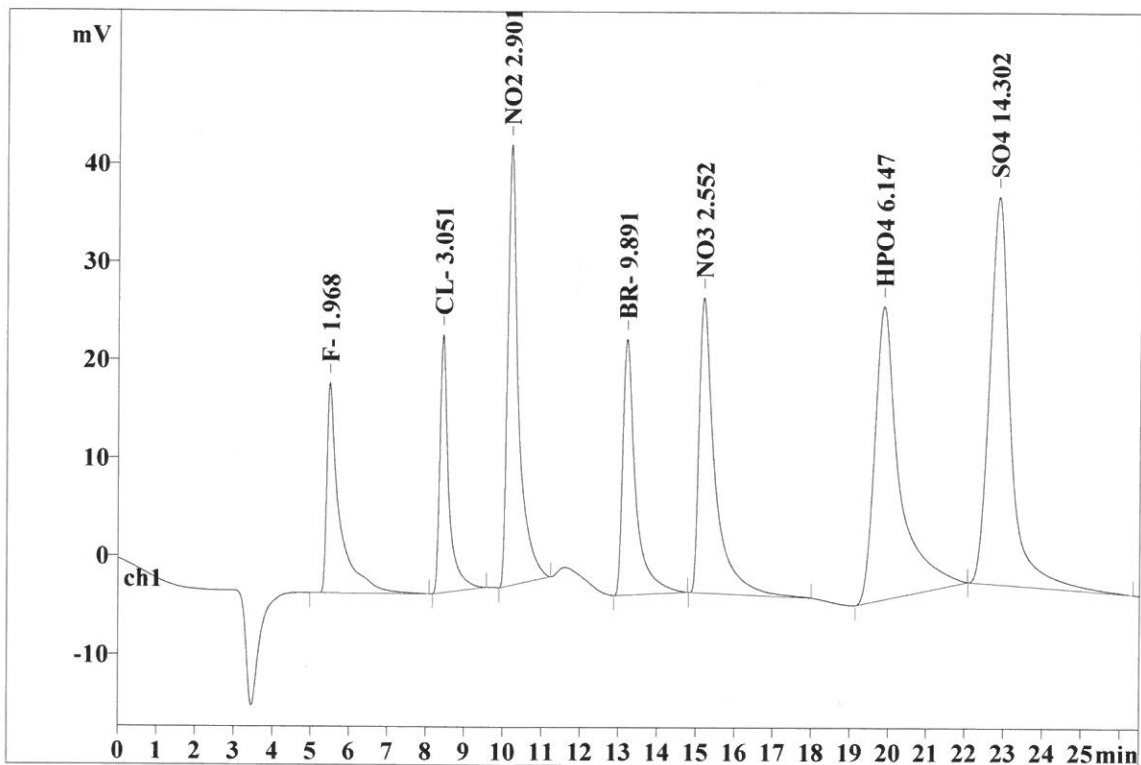

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.49	0.256	21.42	9.81	495.357	8.10
2	8.43	0.208	26.30	12.05	420.117	6.87
3	10.18	0.263	44.96	20.60	888.302	14.52
4	13.20	0.303	26.06	11.94	600.113	9.81
5	15.18	0.375	30.10	13.79	866.246	14.16
6	19.86	0.571	29.89	13.69	1340.539	21.91
7	22.86	0.524	39.54	18.11	1508.497	24.65
7	26.50	0.357	218.24	99.99	6119.172	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:40:00 AM
Printed by: wet


Ident: CCB
Analysis from: 12/20/2019 7:25:41 PM
File: _2019-12-20_

Last save: 12/20/2019 7:52:12 PM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24070

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

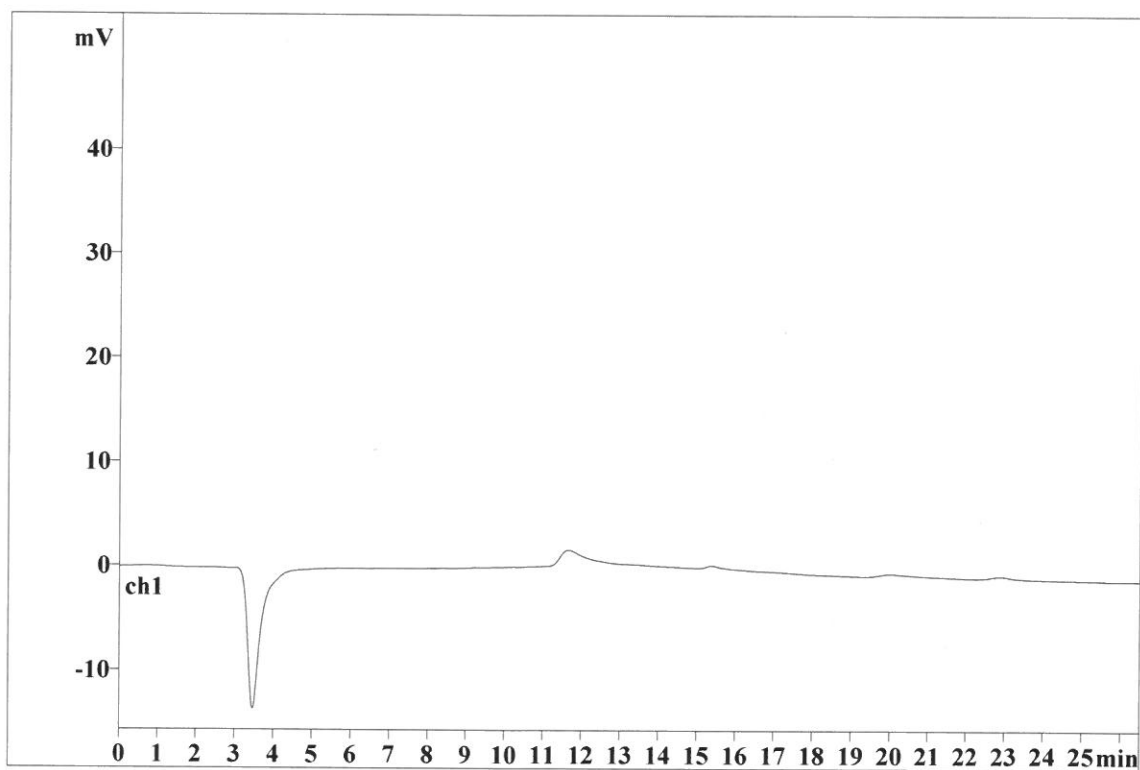

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD