

LB106934

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AL

Instrument ID : Konelab

12/26/2019 13:12

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.553	0.0	0.097	
ICB1	0.734	0.0	0.002	
CCV1	243.610	0.0	0.245	
CCB1	0.563	0.0	0.002	
PB125732BL	0.546	0.0	0.002	
PB125732BS	96.704	0.0	0.098	
K6436-06	1.608	0.0	0.003	
K6436-06DUP	1.523	0.0	0.003	
K6436-06MS	39.996	0.0	0.042	
K6436-06MSD	39.899	0.0	0.042	
K6436-07	1.885	0.0	0.004	
K6437-01	0.679	0.0	0.002	
K6437-02	1.664	0.0	0.003	
K6437-03	2.412	0.0	0.004	
CCV2	238.210	0.0	0.239	
CCB2	0.429	0.0	0.002	
K6437-04	1.349	0.0	0.003	
K6437-05	0.779	0.0	0.003	
K6437-07	1.021	0.0	0.003	
K6437-08	0.604	0.0	0.002	
K6437-06	0.298	0.0	0.002	
CCV3	257.575	0.0	0.259	
CCB3	0.335	0.0	0.002	

N	23
Mean	44.695
SD	84.7956
CV%	189.72

Aquakem v. 7.2AQ1

ae

Results from time period:

Thu Dec 26 12:58:32 2019

Thu Dec 26 13:10:00 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.1662	µg/l	12/26/2019 10:07:30	
5.0PPBCN	A	Total CN	P	5.1777	µg/l	12/26/2019 10:07:31	
10PPBCN	A	Total CN	P	10.1515	µg/l	12/26/2019 10:07:32	
50PPBCN	A	Total CN	P	50.2619	µg/l	12/26/2019 10:07:33	
100PPBCN	A	Total CN	P	101.0775	µg/l	12/26/2019 10:07:34	
250PPBCN	A	Total CN	P	246.8235	µg/l	12/26/2019 10:07:35	
500PPBCN	A	Total CN	P	501.3417	µg/l	12/26/2019 10:07:36	
ICV1	S	Total CN	P	95.5533	µg/l	12/26/2019 12:58:32	
ICB1	S	Total CN	P	0.7343	µg/l	12/26/2019 12:58:33	
CCV1	S	Total CN	P	243.6097	µg/l	12/26/2019 12:58:34	
CCB1	S	Total CN	P	0.563	µg/l	12/26/2019 12:58:35	
PB125732BL	S	Total CN	P	0.5456	µg/l	12/26/2019 12:58:36	
PB125732BS	S	Total CN	P	96.7043	µg/l	12/26/2019 12:58:37	
K6436-06	S	Total CN	P	1.6076	µg/l	12/26/2019 12:58:38	
K6436-06DUP	S	Total CN	P	1.5234	µg/l	12/26/2019 12:58:39	
K6436-06MS	S	Total CN	P	39.9958	µg/l	12/26/2019 12:58:40	
K6436-06MSD	S	Total CN	P	39.899	µg/l	12/26/2019 12:58:41	
K6436-07	S	Total CN	P	1.8855	µg/l	12/26/2019 12:58:42	
K6437-01	S	Total CN	P	0.6786	µg/l	12/26/2019 13:06:07	
K6437-02	S	Total CN	P	1.6635	µg/l	12/26/2019 13:06:08	
K6437-03	S	Total CN	P	2.4122	µg/l	12/26/2019 13:06:09	
CCV2	S	Total CN	P	238.2103	µg/l	12/26/2019 13:06:10	
CCB2	S	Total CN	P	0.4294	µg/l	12/26/2019 13:06:11	
K6437-04	S	Total CN	P	1.3495	µg/l	12/26/2019 13:06:12	
K6437-05	S	Total CN	P	0.7791	µg/l	12/26/2019 13:06:13	
K6437-07	S	Total CN	P	1.0206	µg/l	12/26/2019 13:06:14	
K6437-08	S	Total CN	P	0.6035	µg/l	12/26/2019 13:06:15	
K6437-06	S	Total CN	P	0.298	µg/l	12/26/2019 13:09:58	
CCV3	S	Total CN	P	257.5752	µg/l	12/26/2019 13:09:59	
CCB3	S	Total CN	P	0.3354	µg/l	12/26/2019 13:10:00	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Ab

Instrument ID : Konelab

12/26/2019 13:16


Test Total CN

Accepted 12/26/2019 10:10

Factor 1003
Bias 0.002

Coeff. of det. 0.999936

Errors

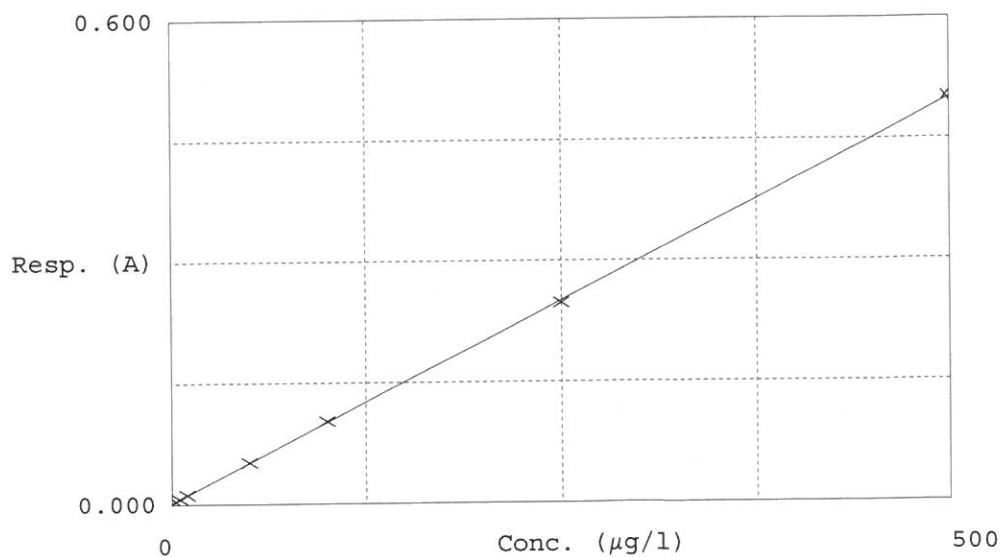

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.1662	0.0000	
2	5.0PPBCN	0.007	5.1777	5.0000	
3	10PPBCN	0.012	10.1515	10.0000	
4	50PPBCN	0.052	50.2619	50.0000	
5	100PPBCN	0.103	101.0775	100.0000	
6	250PPBCN	0.248	246.8235	250.0000	
7	500PPBCN	0.502	501.3417	500.0000	