


LB106975

INSTRUMENT ID CW1

245.1

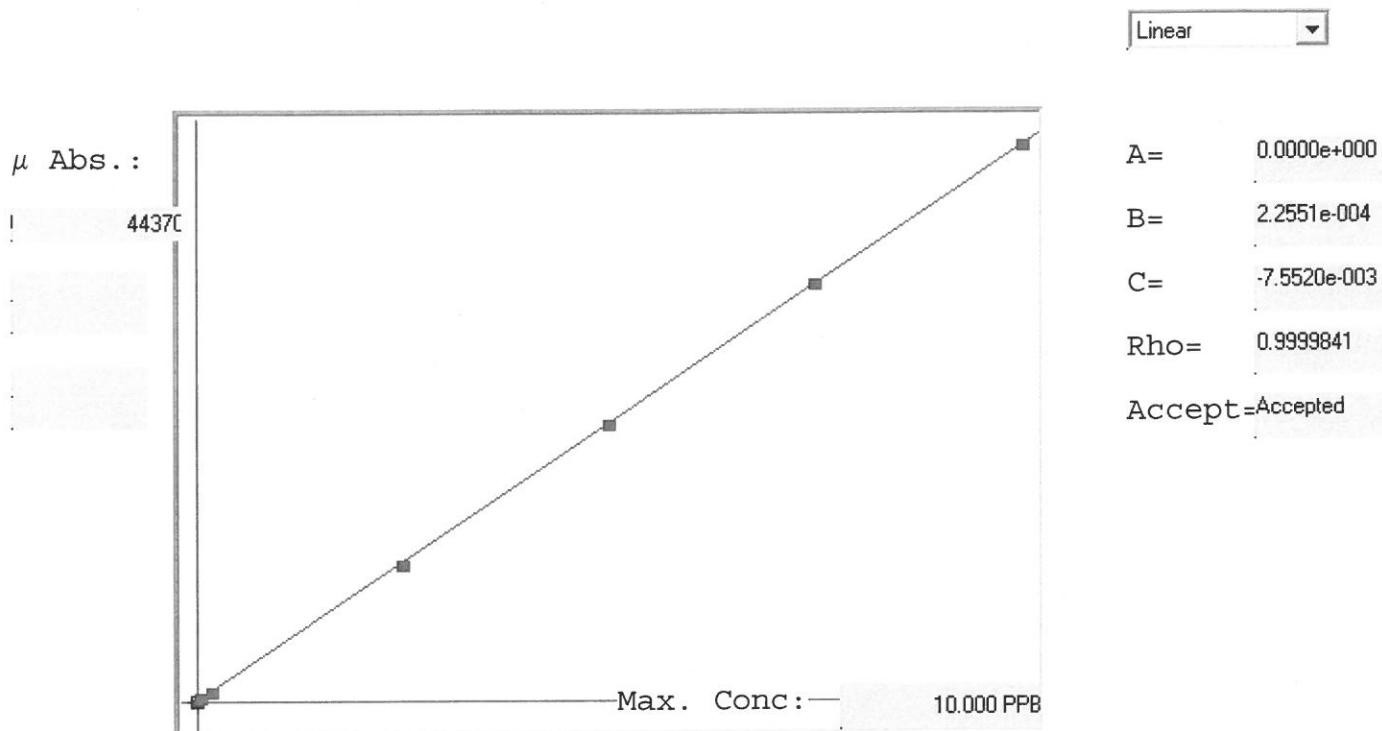

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.021	0.021	125	0.000	125				
0.05	0.050	0.066	0.016	326	0.0 %	326				
0.2	0.200	0.194	-0.006	895	0.0 %	895				
2.5	2.500	2.457	-0.043	10927	0.0 %	10927				
5.0	5.000	4.994	-0.006	22177	0.0 %	22177				
7.5	7.500	7.521	0.021	33383	0.0 %	33383				
10.0	10.000	9.998	-0.002	44370	0.0 %	44370				

LB106975 INSTRUMENT ID CV1

Method: 245.1

Operator: Admin

Date of Analysis: 30 Dec 2019 16:55:24

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	56.0	125	-	0.0000	245.1	PPB	30 Dec 2019 16:56:19	S	Std
0.05 - 1	50.05	326	-	0.0500	245.1	PPB	30 Dec 2019 17:04:12	S	Std
0.2 - 1	50.2	895	-	0.2000	245.1	PPB	30 Dec 2019 17:06:29	S	Std
2.5 - 1	52.5	10927	-	2.5000	245.1	PPB	30 Dec 2019 17:08:46	S	Std
5.0 - 1	55.0	22177	-	5.0000	245.1	PPB	30 Dec 2019 17:11:03	S	Std
7.5 - 1	57.5	33383	-	7.5000	245.1	PPB	30 Dec 2019 17:13:19	S	Std
10.0 - 1	510.0	44370	-	10.0000	245.1	PPB	30 Dec 2019 17:15:35	S	Std
ICV44 - 1	ICV44	18076	4.0688 ✓	-	245.1	PPB	30 Dec 2019 17:24:43	U	SMPL
ICB44 - 1	ICB44	161	0.0288 ✓	-	245.1	PPB	30 Dec 2019 17:26:58	U	SMPL
CCV89 - 1	CCV89	22516	5.0700 ✓	-	245.1	PPB	30 Dec 2019 17:30:43	U	SMPL
CCB89 - 1	CCB89	165	0.0297 ✓	-	245.1	PPB	30 Dec 2019 17:32:58	U	SMPL
CRA - 1	CRA	325	0.0657 ✓	-	245.1	PPB	30 Dec 2019 17:35:14	U	SMPL
HighStd - 1	HighStd	44501	10.0279 ✓	-	245.1	PPB	30 Dec 2019 17:37:29	U	SMPL
ChkStd - 1	ChkStd	30348	6.8362 ✓	-	245.1	PPB	30 Dec 2019 17:39:45	U	SMPL
PB125800BL - 1	PBW	32	-0.0003	-	245.1	PPB	30 Dec 2019 17:42:01	U	SMPL
PB125800BS - 1	LCSW	16626	3.7418 ✓	-	245.1	PPB	30 Dec 2019 17:44:17	U	SMPL
K6348-01 - 1	MW-8	198	0.0371	-	245.1	PPB	30 Dec 2019 17:46:35	U	SMPL
K6348-01DUP - 1	MW-8DUP	175	0.0319	-	245.1	PPB	30 Dec 2019 17:48:52	U	SMPL
K6348-01MS - 1	MW-8MS	18940	4.2636 ✓	-	245.1	PPB	30 Dec 2019 17:51:09	U	SMPL
K6348-01MSD - 1	MW-8MSD	18719	4.2138 ✓	-	245.1	PPB	30 Dec 2019 17:53:26	U	SMPL
K6434-03 - 1	GW-1-DISCHARGE	190	0.0353	-	245.1	PPB	30 Dec 2019 17:55:42	U	SMPL
CCV90 - 1	CCV90	22529	5.0730 ✓	-	245.1	PPB	30 Dec 2019 17:57:57	U	SMPL
CCB90 - 1	CCB90	166	0.0299 ✓	-	245.1	PPB	30 Dec 2019 18:00:13	U	SMPL
K6348-01LX5 - 1		45	0.0026 ✓	-	245.1	PPB	30 Dec 2019 18:02:28	U	SMPL
K6348-01A - 1		17484	3.9353 ✓	-	245.1	PPB	30 Dec 2019 18:04:44	U	SMPL
CCV91 - 1	CCV91	22509	5.0684 ✓	-	245.1	PPB	30 Dec 2019 18:07:00	U	SMPL
CCB91 - 1	CCB91	71	0.0085 ✓	-	245.1	PPB	30 Dec 2019 18:09:15	U	SMPL