


LB107081
INSTRUMENT 10 CV1

7471B

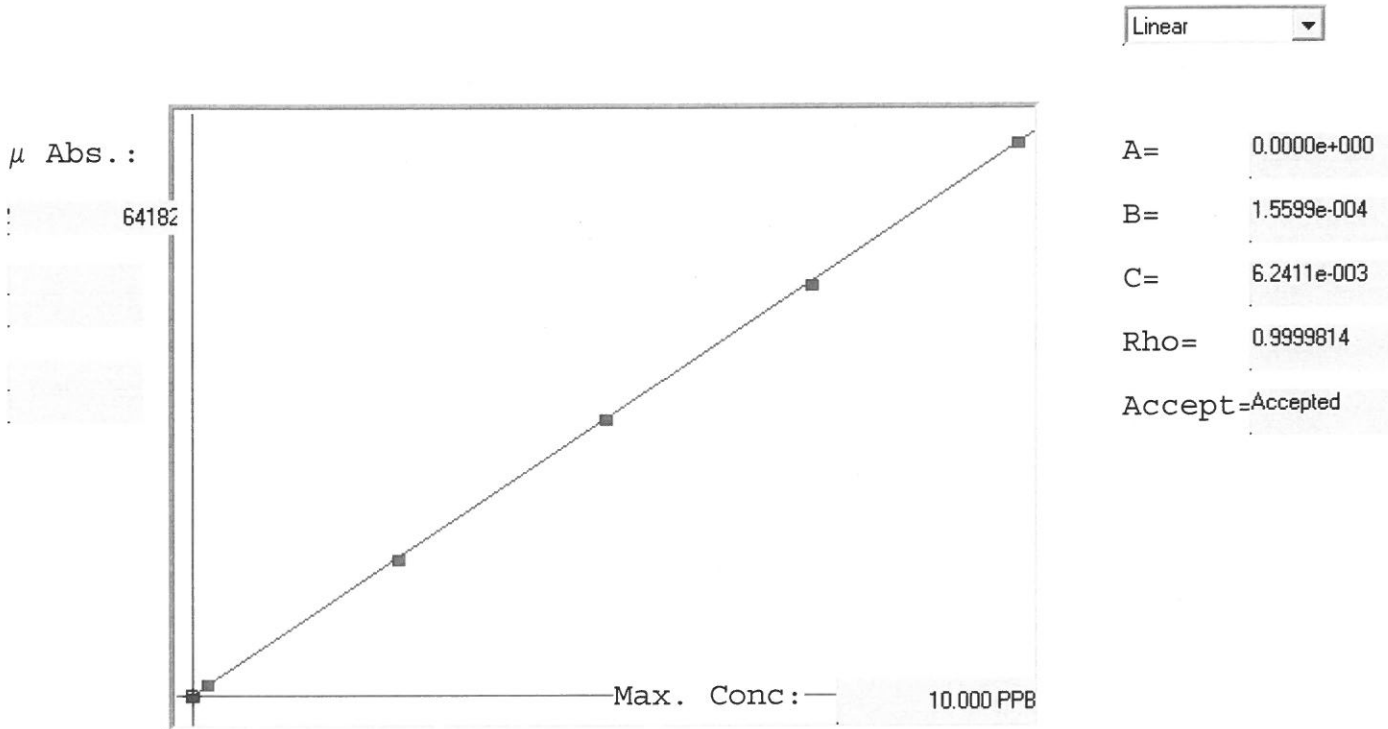

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.026	-0.026	-209	0.000	-209				
0.2	0.200	0.227	0.027	1415	0.0 %	1415				
2.5	2.500	2.504	0.004	16012	0.0 %	16012				
5.0	5.000	5.012	0.012	32088	0.0 %	32088				
7.5	7.500	7.466	-0.034	47824	0.0 %	47824				
10.0	10.000	10.018	0.018	64182	0.0 %	64182				

LB107031 INSTRUMENT ID CV1

Method: 7471B		Operator: Admin		Date of Analysis: 06 Jan 2020 08:28:45					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1		-209	-	0.0007471B		PPB	06 Jan 2020 08:47:23	S	Std
0.2 - 1		1415	-	0.2007471B		PPB	06 Jan 2020 08:49:40	S	Std
2.5 - 1		16012	-	2.5007471B		PPB	06 Jan 2020 08:51:56	S	Std
5.0 - 1		32088	-	5.0007471B		PPB	06 Jan 2020 08:54:13	S	Std
7.5 - 1		47824	-	7.5007471B		PPB	06 Jan 2020 08:56:29	S	Std
10.0 - 1		64182	-	10.0007471B		PPB	06 Jan 2020 08:58:45	S	Std
ICV50 - 1	ICV50	24149	3.7732 ✓	-7471B		PPB	06 Jan 2020 09:01:45	U	SMPL
ICB50 - 1	ICB50	-118	-0.0122 ✓	-7471B		PPB	06 Jan 2020 09:04:00	U	SMPL
CCV12 - 1	CCV12	32401	5.0604 ✓	-7471B		PPB	06 Jan 2020 09:06:14	U	SMPL
CCB12 - 1	CCB12	-117	-0.0120 ✓	-7471B		PPB	06 Jan 2020 09:08:30	U	SMPL
CRA - 1	CRA	1509	0.2416 ✓	-7471B		PPB	06 Jan 2020 09:10:44	U	SMPL
HighStd - 1	HighStd	64103	10.0055 ✓	-7471B		PPB	06 Jan 2020 09:12:59	U	SMPL
ChkStd - 1	ChkStd	44031	6.8745 ✓	-7471B		PPB	06 Jan 2020 09:15:14	U	SMPL
PB125900BL - 1	PBS	-113	-0.0114 ✓	-7471B		PPB	06 Jan 2020 09:17:31	U	SMPL
PB125900BS - 1	LCSS	24160	3.7749 ✓	-7471B		PPB	06 Jan 2020 09:19:47	U	SMPL
L1001-01 - 1	PAMT-RORO-CORE-3-12-30-19	23954	3.7428 ✓	-7471B		PPB	06 Jan 2020 09:22:03	U	SMPL
L1001-02 - 1	RAMT-RORO-COMP-1-12-30-19	7738	1.2133 ✓	-7471B		PPB	06 Jan 2020 09:24:20	U	SMPL
L1001-03 - 1	SC-CORE-3-12-31-19	8086	1.2676 ✓	-7471B		PPB	06 Jan 2020 09:26:36	U	SMPL
L1001-04 - 1	SC-1-12-31-19	7000	1.0981 ✓	-7471B		PPB	06 Jan 2020 09:28:53	U	SMPL
L1001-05 - 1	PAMT-COMP-1-12-31-19	5456	0.8573 ✓	-7471B		PPB	06 Jan 2020 09:31:08	U	SMPL
CCV13 - 1	CCV13	32171	5.0245 ✓	-7471B		PPB	06 Jan 2020 09:33:23	U	SMPL
CCB13 - 1	CCB13	-73	-0.0051 ✓	-7471B		PPB	06 Jan 2020 09:35:38	U	SMPL
L1001-05DUP - 1	PAMT-COMP-1-12-31-19DUP	5524	0.8679 ✓	-7471B		PPB	06 Jan 2020 09:37:53	U	SMPL
L1001-06 - 1	L1001-05MS	29156	4.5542 ✓	-7471B		PPB	06 Jan 2020 09:44:51	U	SMPL
L1001-07 - 1	L1001-05MSD	29123	4.5490 ✓	-7471B		PPB	06 Jan 2020 09:47:07	U	SMPL
L1001-08 - 1	PAMT-COMP-2-12-31-19	5904	0.9272 ✓	-7471B		PPB	06 Jan 2020 09:49:22	U	SMPL
L1008-01 - 1	CL-02-010220	2125	0.3377 ✓	-7471B		PPB	06 Jan 2020 09:51:38	U	SMPL
L1009-01 - 1	NB-08-010220	1487	0.2382 ✓	-7471B		PPB	06 Jan 2020 09:53:54	U	SMPL
L1010-01 - 1	OK-01-010220	4577	0.7202 ✓	-7471B		PPB	06 Jan 2020 09:56:10	U	SMPL
L1011-02 - 1	MC-010220-0-2-COMP-B3	90461	14.1170 ✓	-7471B		PPB	06 Jan 2020 09:58:27	U	SMPL
L1011-04 - 1	MC-010220-2-5-COMP-B3	136887	21.3588 ✓	-7471B		PPB	06 Jan 2020 10:00:44	U	SMPL
L1011-06 - 1	MC-010220-0-2-COMP-B7	77371	12.0751 ✓	-7471B		PPB	06 Jan 2020 10:03:01	U	SMPL
CCV14 - 1	CCV14	32188	5.0271 ✓	-7471B		PPB	06 Jan 2020 10:05:19	U	SMPL
CCB14 - 1	CCB14	-99	-0.0092 ✓	-7471B		PPB	06 Jan 2020 10:07:35	U	SMPL
L1011-08 - 1	MC-010220-2-5-COMP-B7	87154	13.6011 ✓	-7471B		PPB	06 Jan 2020 10:09:50	U	SMPL
L1028-01 - 1	NORTH-BERGEN	23155	3.6181 ✓	-7471B		PPB	06 Jan 2020 10:12:06	U	SMPL
L1001-05LX5 - 1		699	0.1153 ✓	-7471B		PPB	06 Jan 2020 10:14:23	U	SMPL
L1011-02DLX2 - 1		45137	7.0470 ✓	-7471B		PPB	06 Jan 2020 10:16:38	U	SMPL
L1011-04DLX3 - 1		45518	7.1065 ✓	-7471B		PPB	06 Jan 2020 10:18:54	U	SMPL
L1011-06DLX2 - 1		37132	5.7983 ✓	-7471B		PPB	06 Jan 2020 10:21:11	U	SMPL
L1011-08DLX2 - 1		40506	6.3246 ✓	-7471B		PPB	06 Jan 2020 10:23:27	U	SMPL
CCV15 - 1	CCV15	32739	5.1131 ✓	-7471B		PPB	06 Jan 2020 10:25:44	U	SMPL
CCB15 - 1	CCB15	-94	-0.0084 ✓	-7471B		PPB	06 Jan 2020 10:28:01	U	SMPL